

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121625\
 Data File : PD091607.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2025 16:29
 Operator : AR\AJ
 Sample : Q3530-07
 Misc : TOX LOD 50PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 05:02:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX120825.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 12:41:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.869	76241725	1004.9E6	22.288	24.082
7) SA Decachlor...	9.059	8.054	124.5E6	1190.3E6	24.475	25.654
Target Compounds						
2) Toxaphene-1	6.232	5.460	3327852	22445888	68.255	59.934
3) Toxaphene-2	6.431	5.631	3515830	12911684	57.166	51.733
4) Toxaphene-3	7.137	6.740	5490802	55714342	50.194	45.355
5) Toxaphene-4	7.553	7.181	6127449	38464504	44.691	48.561
6) Toxaphene-5	7.918	7.313	3794163	24257551	47.557	42.275


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121625\
Data File : PD091607.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2025 16:29
Operator : AR\AJ
Sample : Q3530-07
Misc : TOX LOD 50PPB
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 05:02:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX120825.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 12:41:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

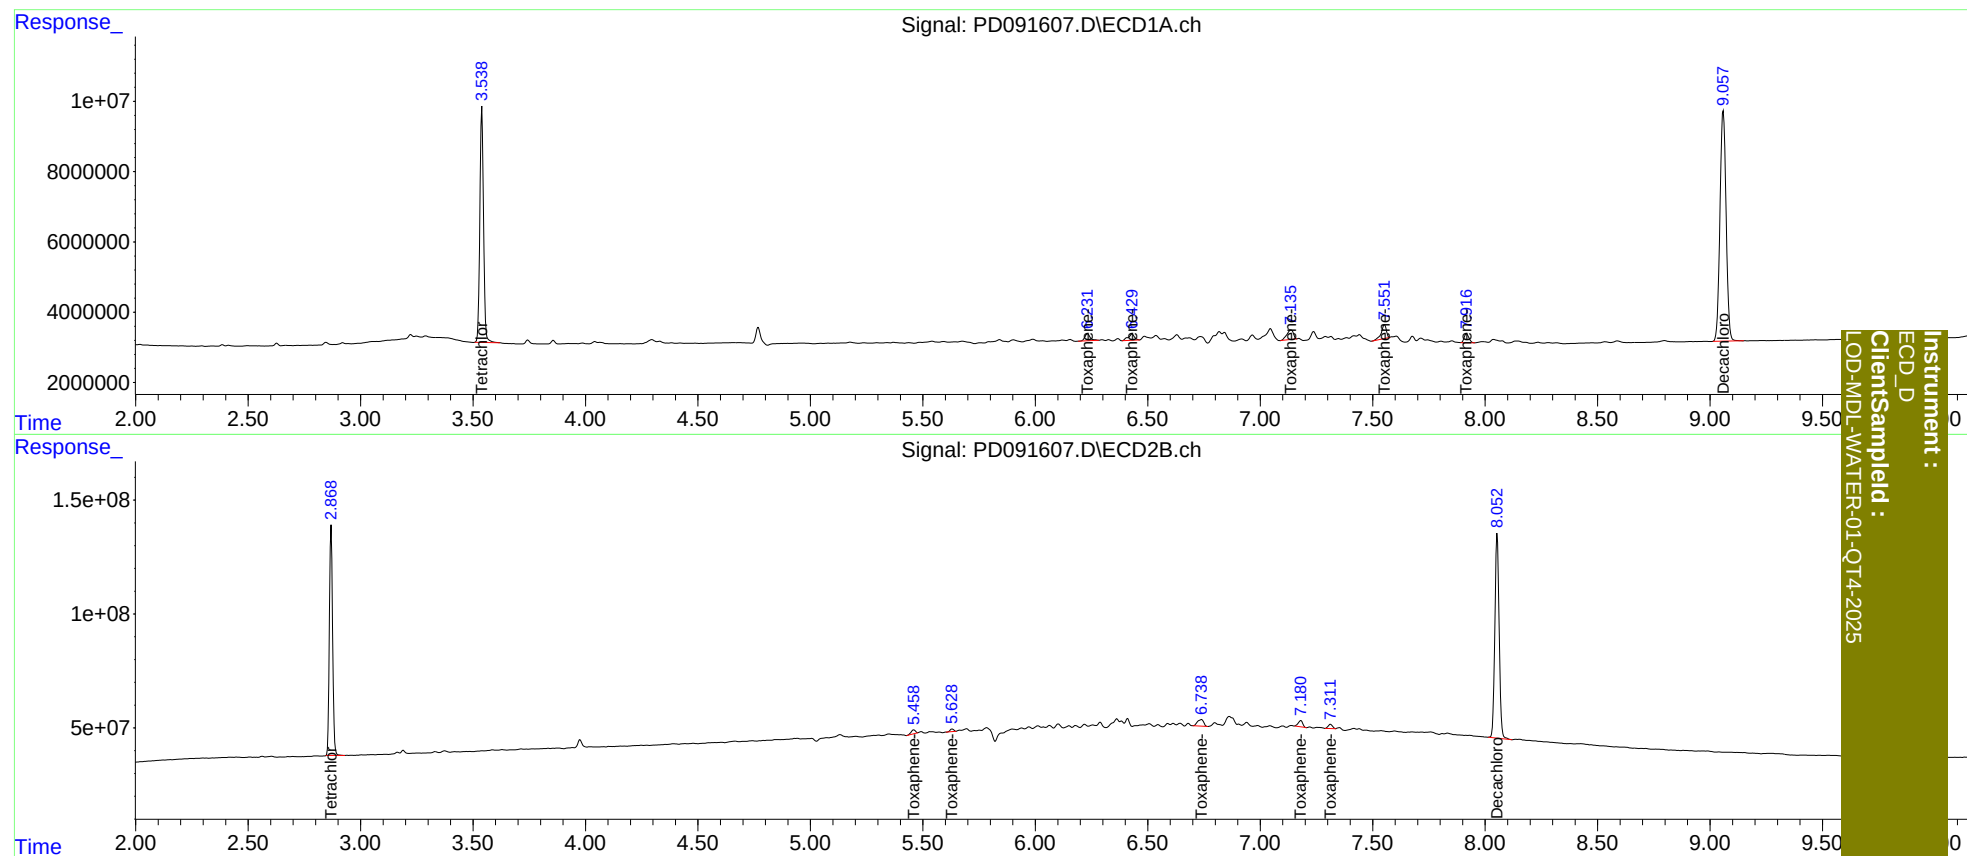


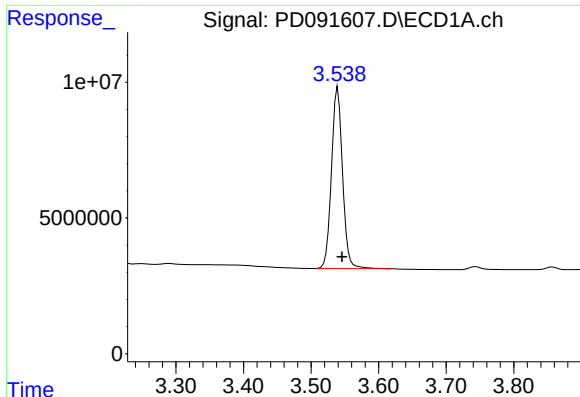

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: -0.006 min
Response: 76241725
Conc: 22.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

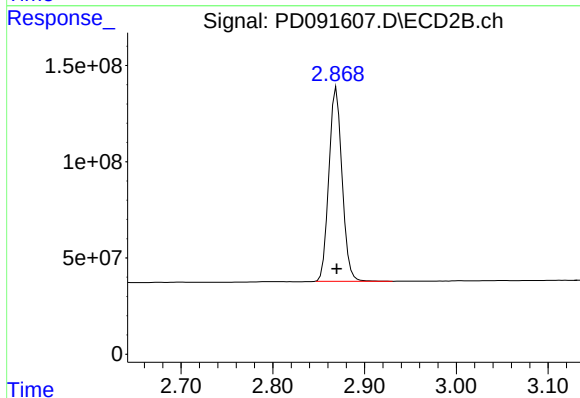


#1 Tetrachloro-m-xylene

R.T.: 2.869 min
Delta R.T.: 0.000 min
Response: 1004851976
Conc: 24.08 ng/ml

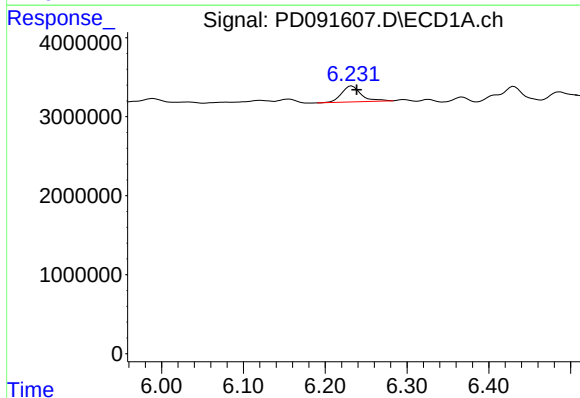


#2 Toxaphene-1

R.T.: 6.232 min
Delta R.T.: -0.006 min
Response: 3327852
Conc: 68.25 ng/ml

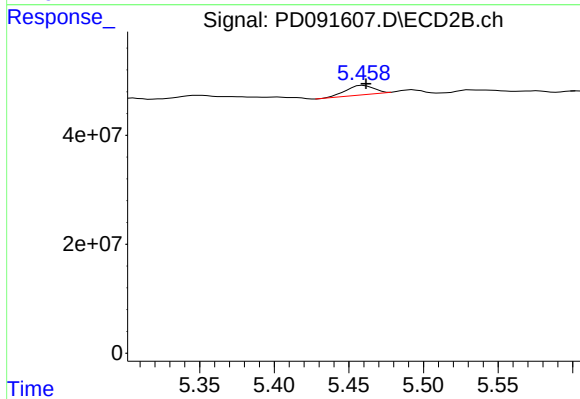

#2 Toxaphene-1


R.T.: 5.460 min
Delta R.T.: -0.002 min
Response: 22445888
Conc: 59.93 ng/ml

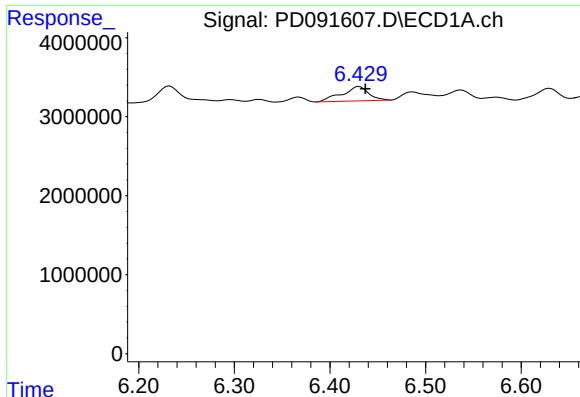

#3 Toxaphene-2


R.T.: 6.431 min
Delta R.T.: -0.007 min
Response: 3515830
Conc: 57.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

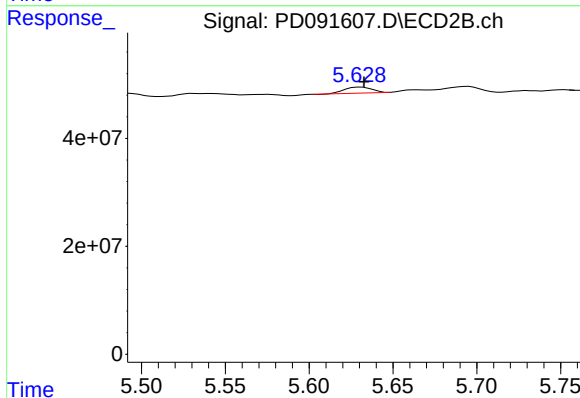


#3 Toxaphene-2

R.T.: 5.631 min
Delta R.T.: -0.002 min
Response: 12911684
Conc: 51.73 ng/ml

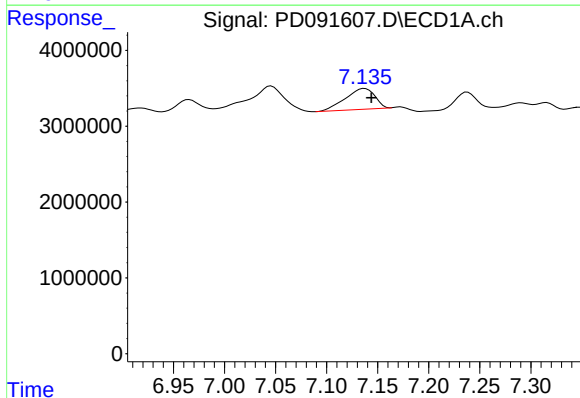


#4 Toxaphene-3

R.T.: 7.137 min
Delta R.T.: -0.006 min
Response: 5490802
Conc: 50.19 ng/ml

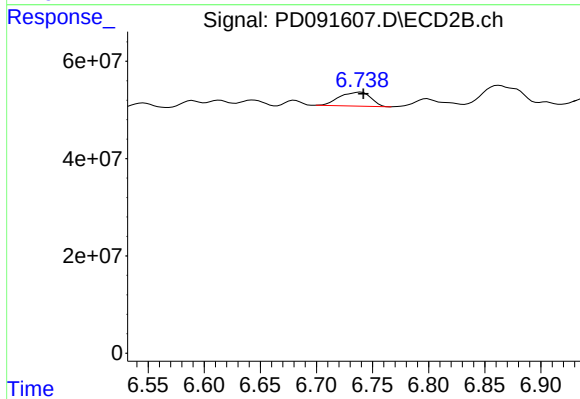

#4 Toxaphene-3


R.T.: 6.740 min
Delta R.T.: -0.002 min
Response: 55714342
Conc: 45.35 ng/ml

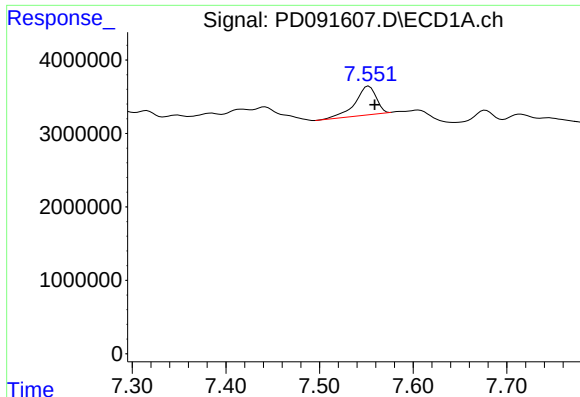

#5 Toxaphene-4


R.T.: 7.553 min
Delta R.T.: -0.006 min
Response: 6127449
Conc: 44.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

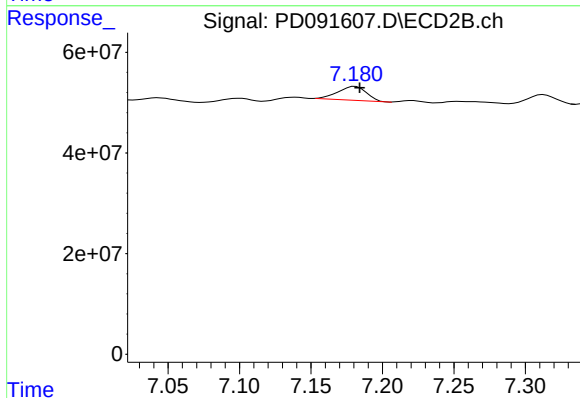


#5 Toxaphene-4

R.T.: 7.181 min
Delta R.T.: -0.003 min
Response: 38464504
Conc: 48.56 ng/ml

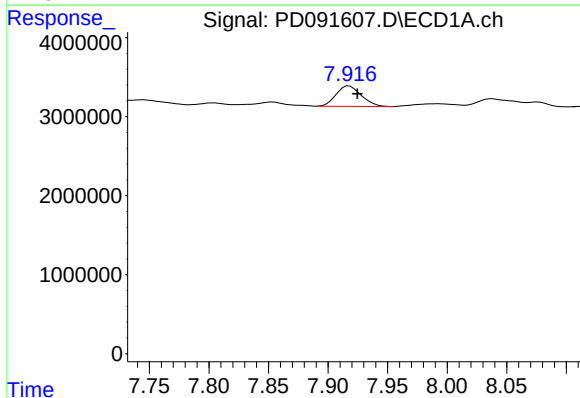


#6 Toxaphene-5

R.T.: 7.918 min
Delta R.T.: -0.007 min
Response: 3794163
Conc: 47.56 ng/ml

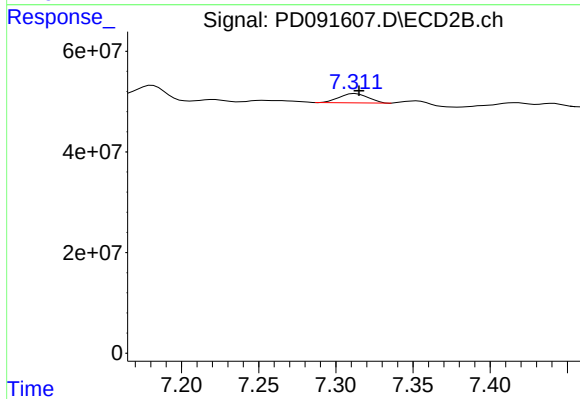

#6 Toxaphene-5


R.T.: 7.313 min
Delta R.T.: -0.002 min
Response: 24257551
Conc: 42.28 ng/ml

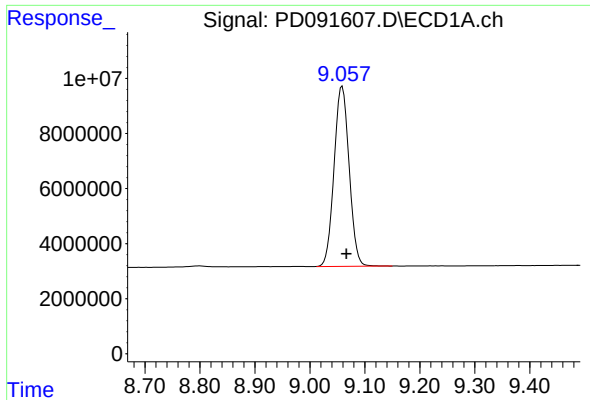

#7 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: -0.008 min
Response: 124532562
Conc: 24.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT4-2025

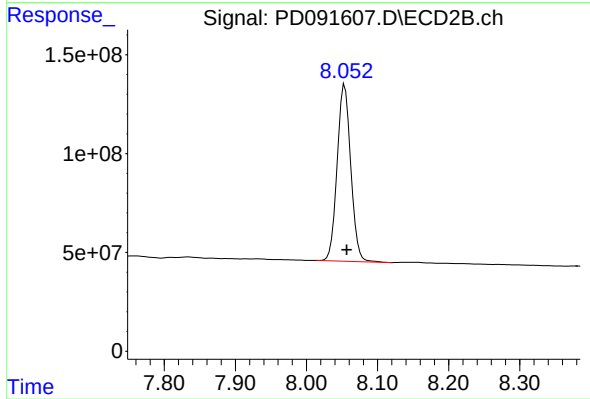

#7 Decachlorobiphenyl

R.T.: 8.054 min
Delta R.T.: -0.003 min
Response: 1190260736
Conc: 25.65 ng/ml