

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121625\
 Data File : PD091622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2025 20:52
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 05:02:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX120825.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 12:41:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.871	139.4E6	1741.3E6	40.747	41.733
7) SA Decachlor...	9.056	8.054	206.3E6	2042.0E6	40.543	44.013
Target Compounds						
2) Toxaphene-1	6.231	5.460	22567401	173.9E6	462.860	464.374
3) Toxaphene-2	6.430	5.631	25332656	107.6E6	411.901	431.214
4) Toxaphene-3	7.137	6.739	45459352	550.0E6	415.562	447.766
5) Toxaphene-4	7.552	7.182	56368255	351.6E6	411.125	443.922
6) Toxaphene-5	7.917	7.313	33125475	265.7E6	415.201	463.086

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121625\
Data File : PD091622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2025 20:52
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 05:02:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX120825.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 12:41:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

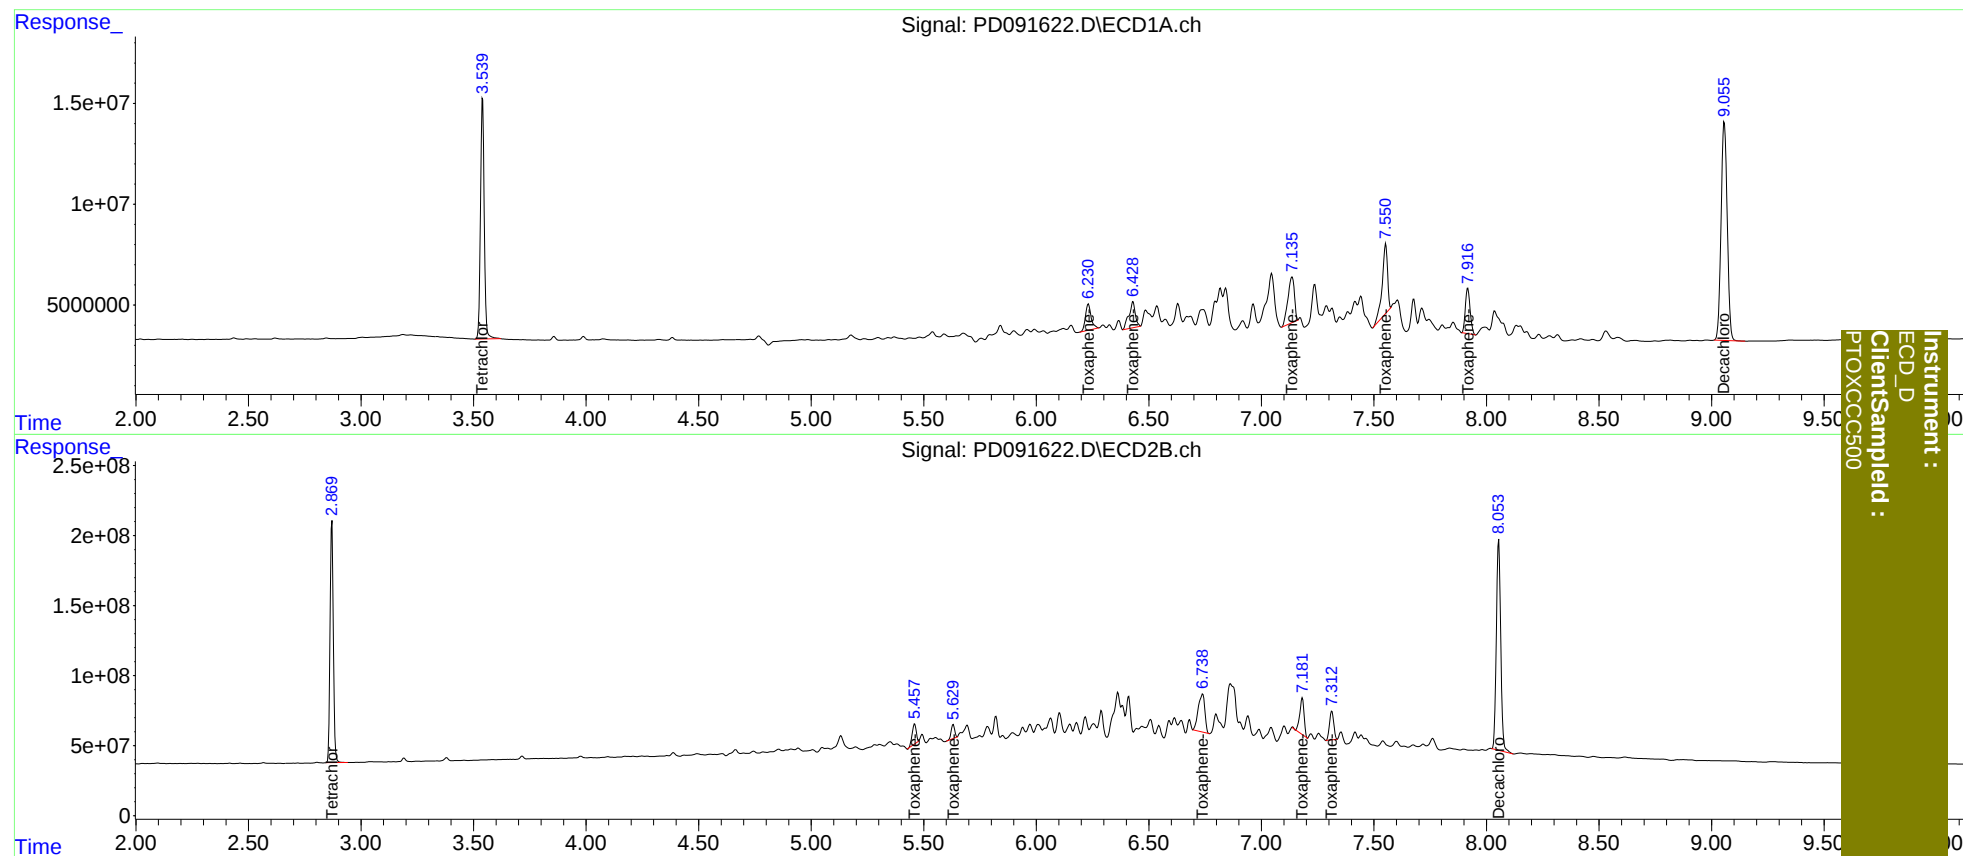

Instrument :
ECD_D
ClientSample :
PTOXCCC500