

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
 Data File : PD056481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 08:55
 Operator : SG\AJ
 Sample : PIBLK17
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:38:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.287	3.961	18168821	30664001	21.938	25.505
27) SA Decachlor...	7.964	8.998	36797272	52064316	40.751	43.273
Target Compounds						
6) B beta-BHC	0.000	4.847f	0	483165	N.D.	0.586


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
Data File : PD056481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 08:55
Operator : SG\AJ
Sample : PIBLK17
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:38:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

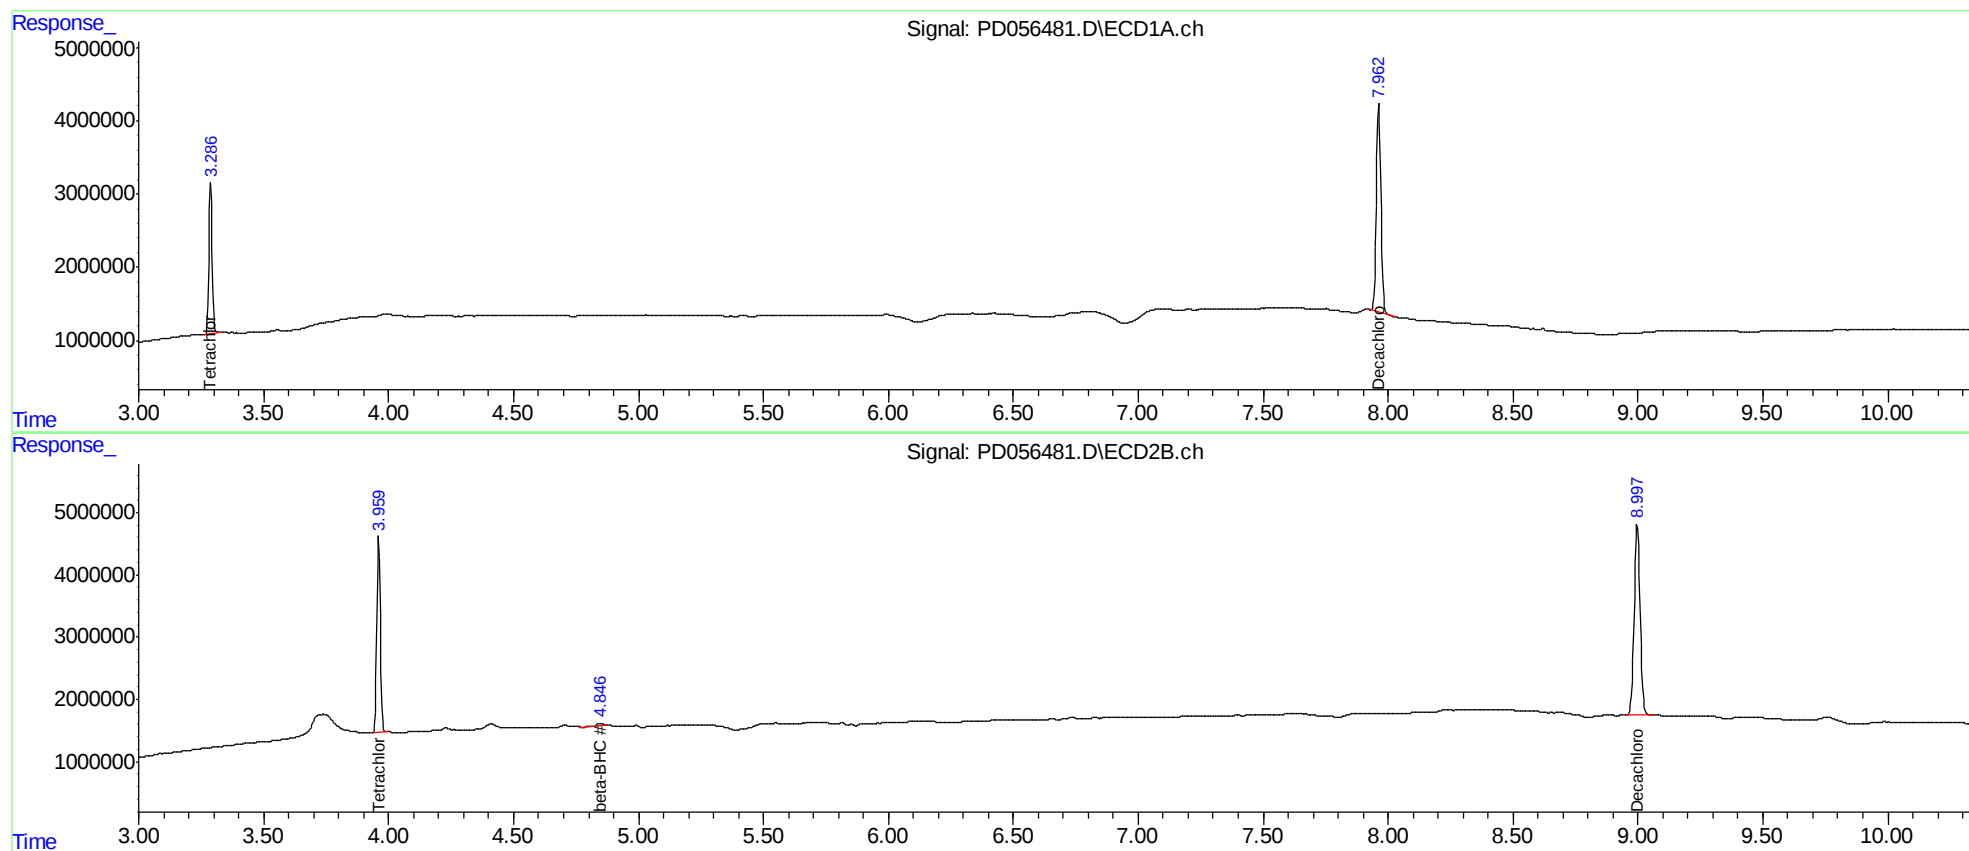


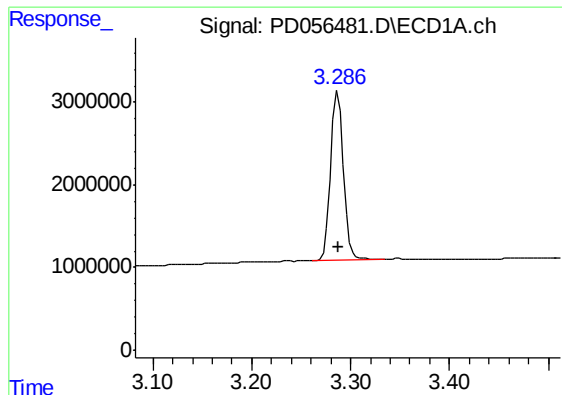

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: 0.000 min
Response: 18168821
Conc: 21.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK17

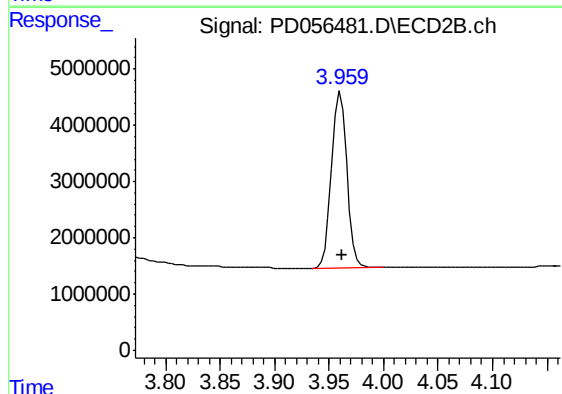


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.002 min
Response: 30664001
Conc: 25.51 ng/ml

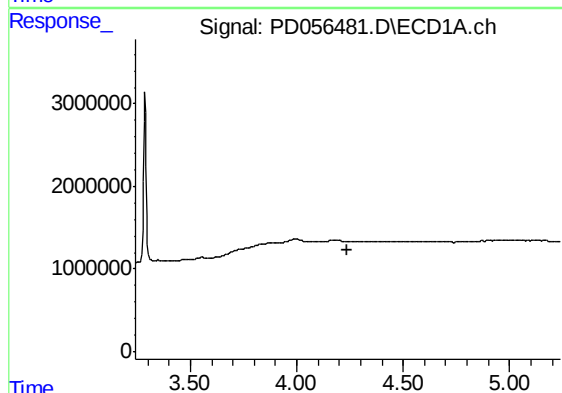


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

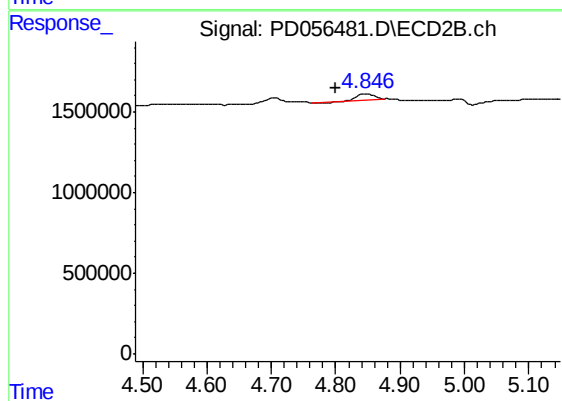

#6 beta-BHC


R.T.: 4.847 min
Delta R.T.: 0.046 min
Response: 483165
Conc: 0.59 ng/ml

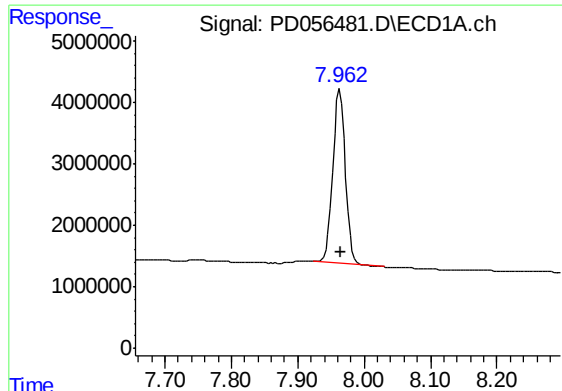

#27 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: -0.002 min
Response: 36797272
Conc: 40.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK17

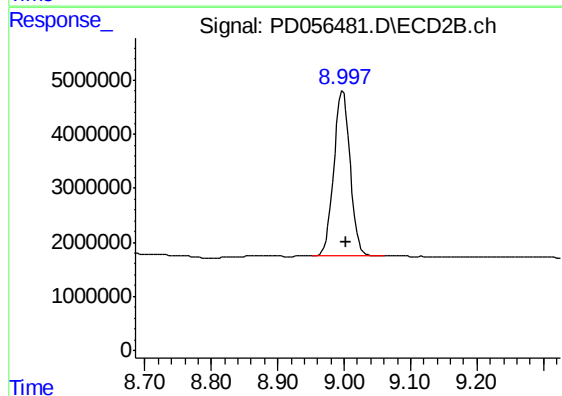

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: -0.005 min
Response: 52064316
Conc: 43.27 ng/ml