

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
 Data File : PD056487.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 10:41
 Operator : SG\AJ
 Sample : PB125487BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK87

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:40:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.961	18302493	31598088	22.099	26.282
27)	SA Decachlor...	7.961	8.998	37803889	53609789	41.866	44.558
Target Compounds							
7)	B delta-BHC	0.000	4.991f	0	1143916	N.D.	0.687
19)	B Endosulfa...	0.000	7.240	0	4330013	N.D.	3.238


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
Data File : PD056487.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 10:41
Operator : SG\AJ
Sample : PB125487BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PBLK87

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:40:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

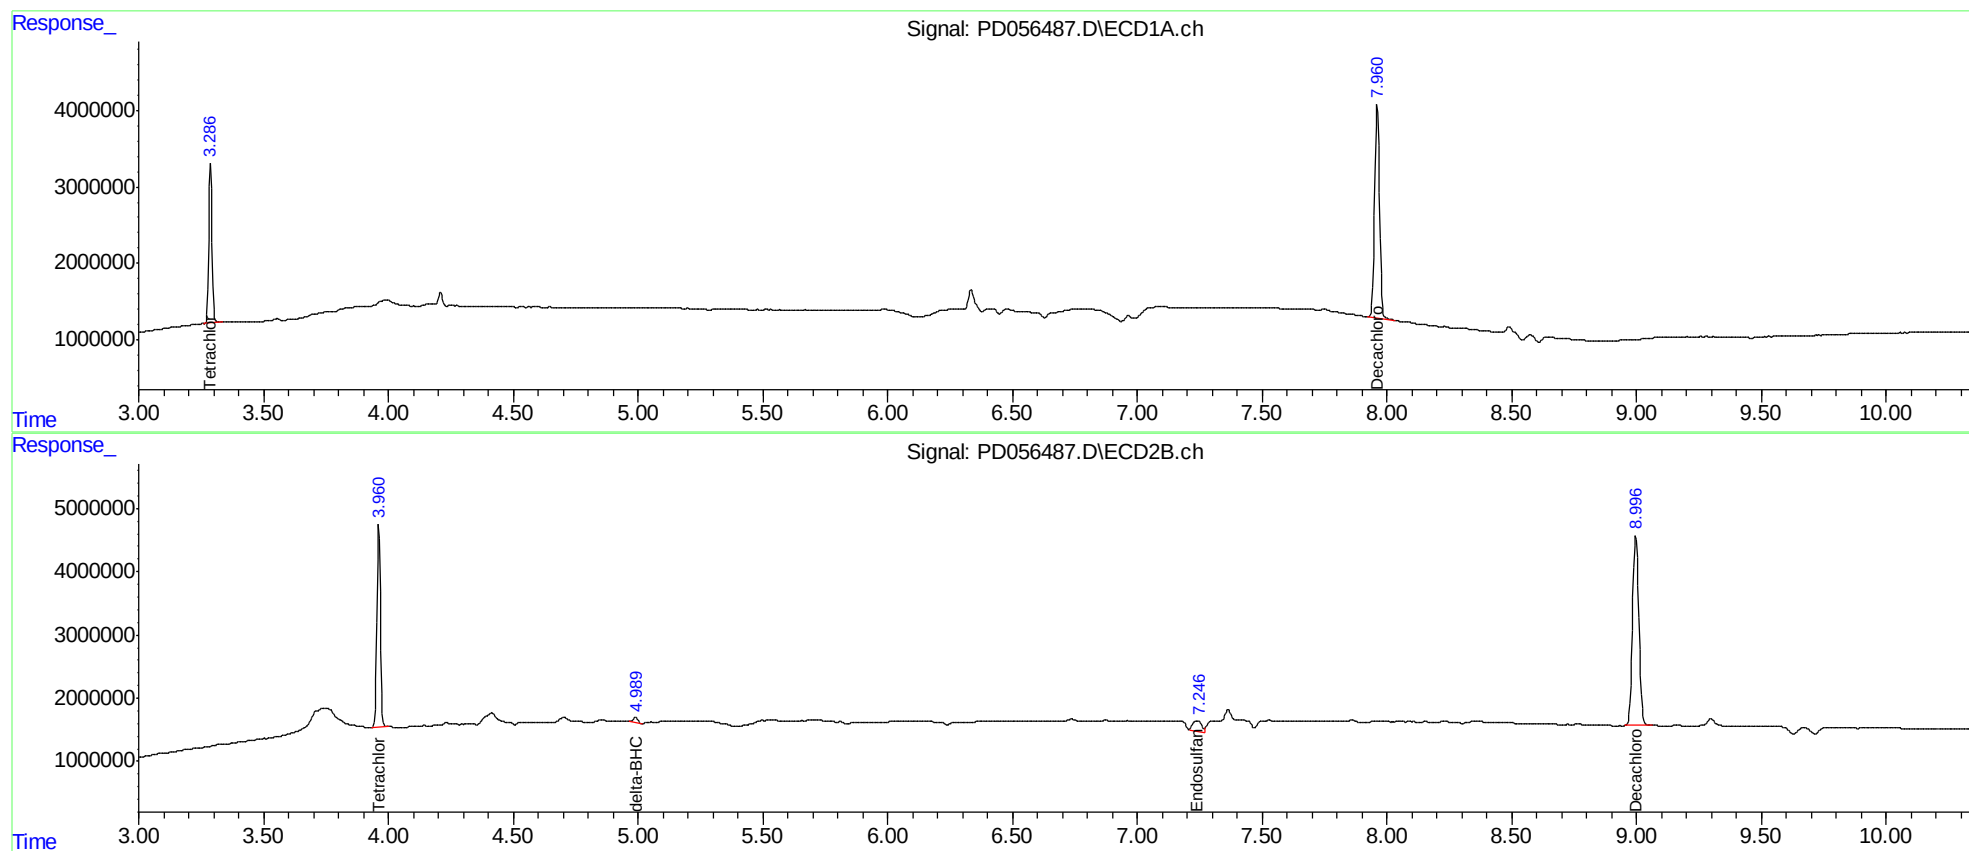


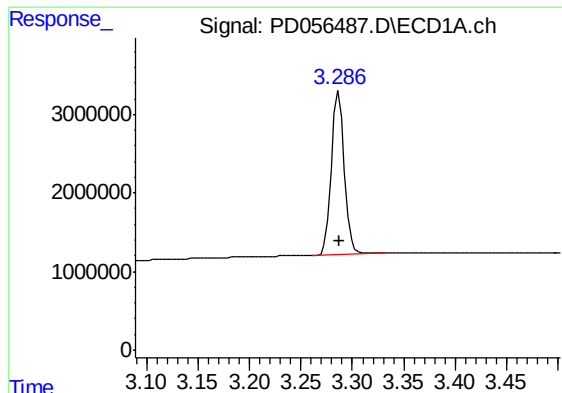

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: -0.001 min
Response: 18302493
Conc: 22.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK87

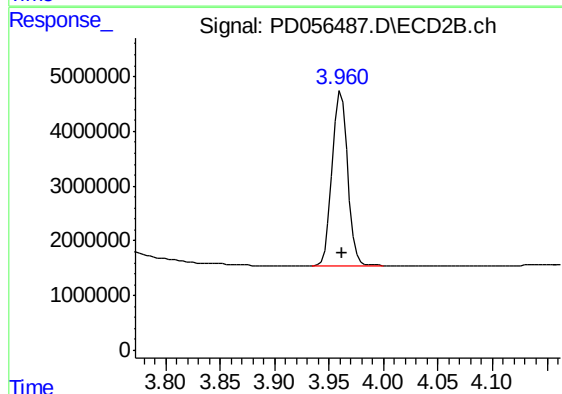


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.001 min
Response: 31598088
Conc: 26.28 ng/ml

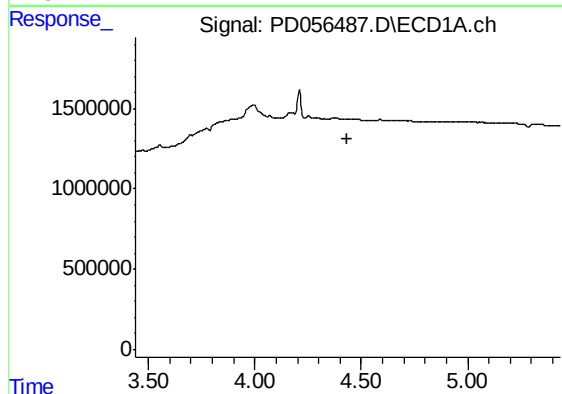


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

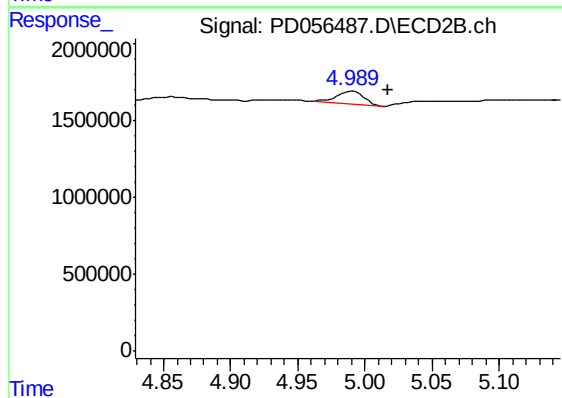

#7 delta-BHC


R.T.: 4.991 min
Delta R.T.: -0.026 min
Response: 1143916
Conc: 0.69 ng/ml

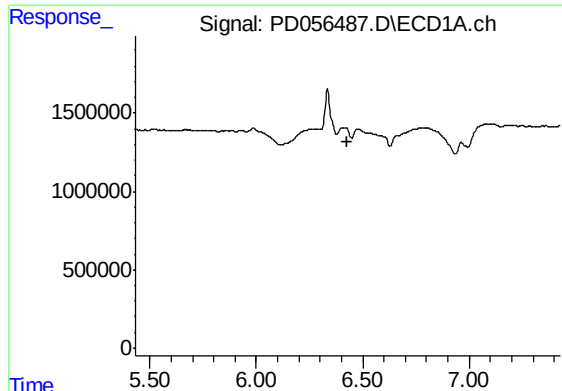

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK87

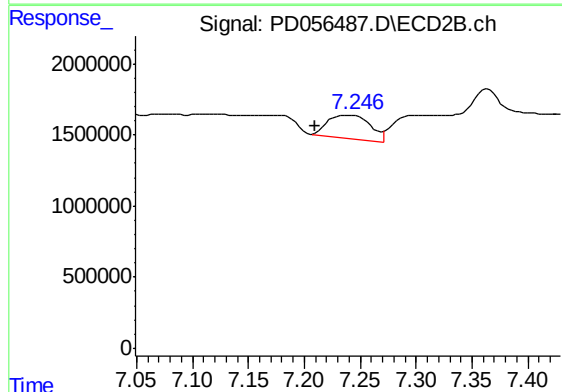


#19 Endosulfan Sulfate

R.T.: 7.240 min
Delta R.T.: 0.030 min
Response: 4330013
Conc: 3.24 ng/ml

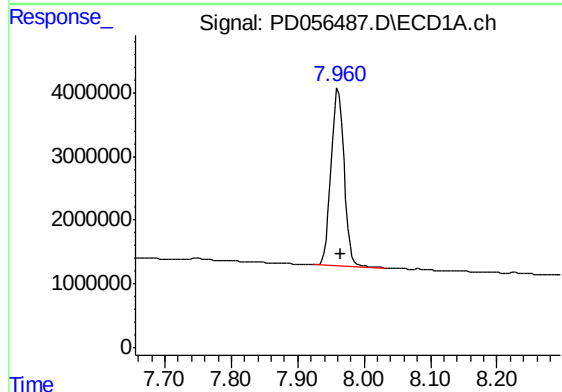

#27 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.004 min
Response: 37803889
Conc: 41.87 ng/ml

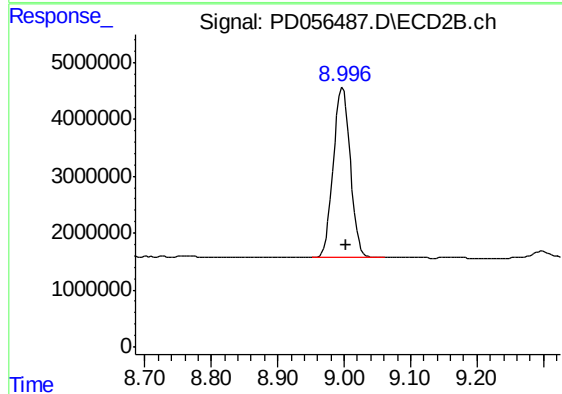

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: -0.005 min
Response: 53609789
Conc: 44.56 ng/ml