

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
 Data File : PD056490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 11:55
 Operator : SG\AJ
 Sample : K6253-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0C09

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:41:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.962	16489263	28462454	19.910	23.674
27)	SA Decachlor...	7.962	8.999	25754789	36383374	28.522	30.240
Target Compounds							
10)	B trans-Chl...	0.000	5.998f	0	3999034	N.D.	2.419


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
Data File : PD056490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 11:55
Operator : SG\AJ
Sample : K6253-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0C09

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:41:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

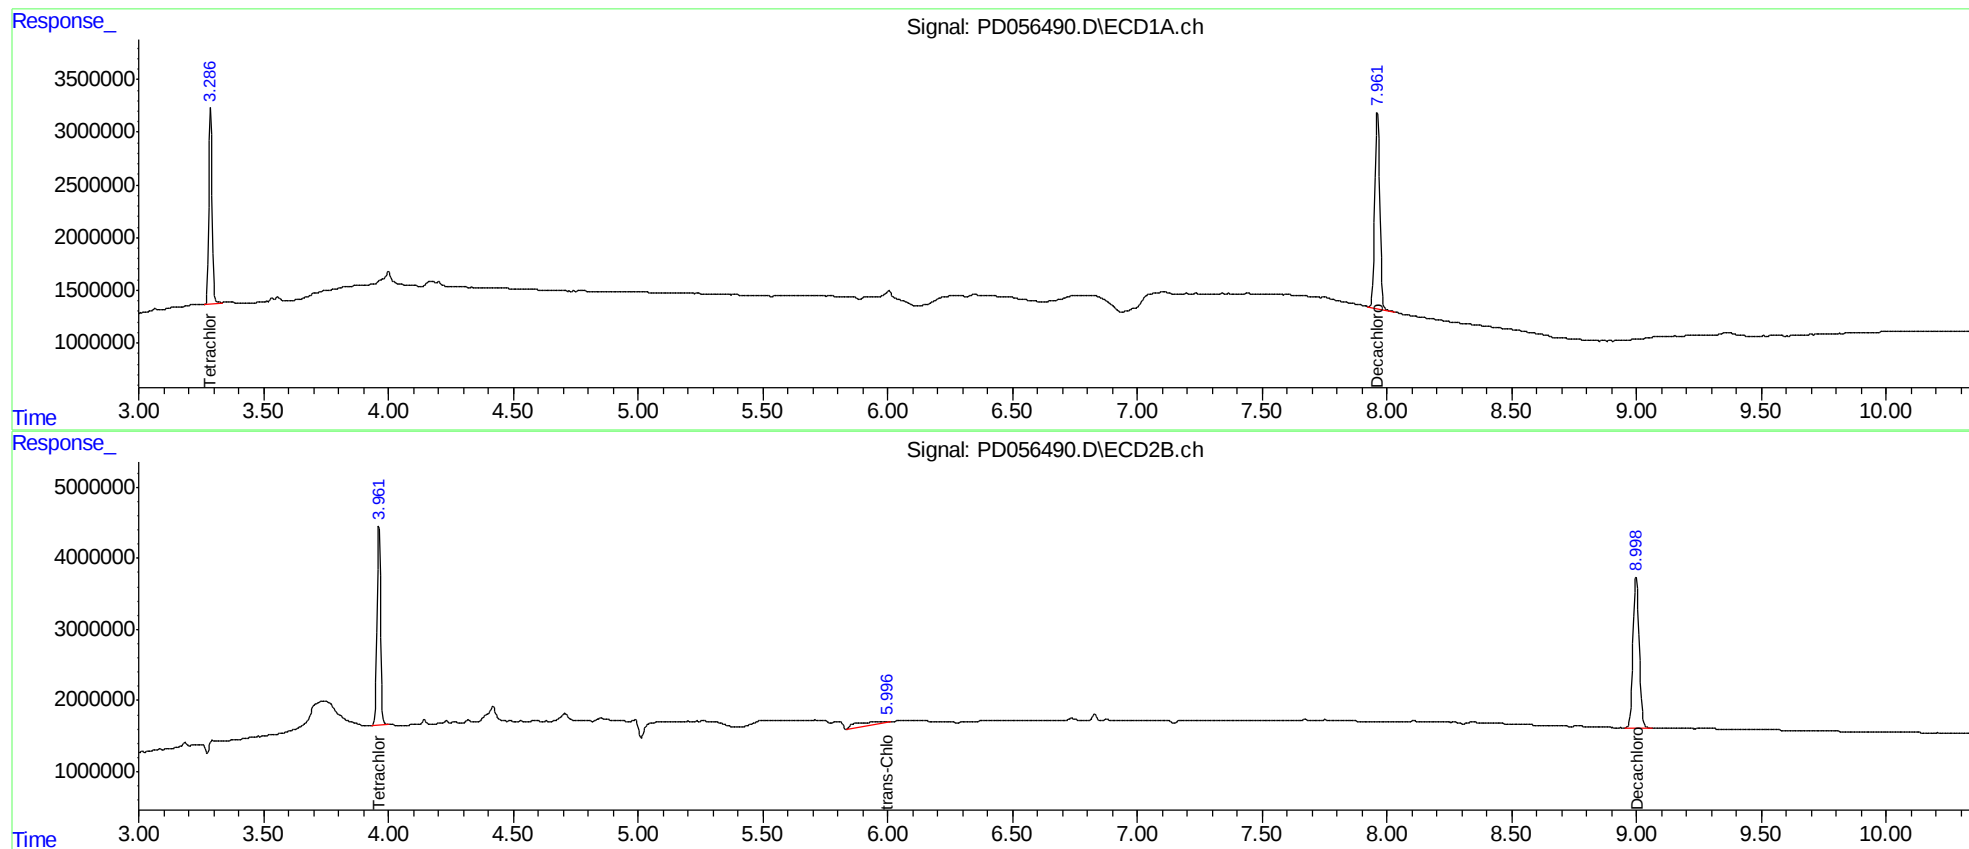


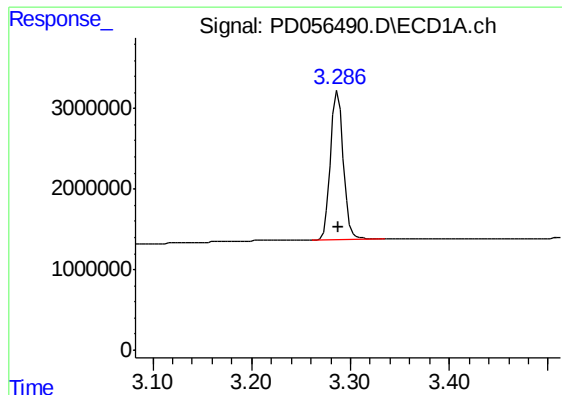

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: 0.000 min
Response: 16489263
Conc: 19.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0C09

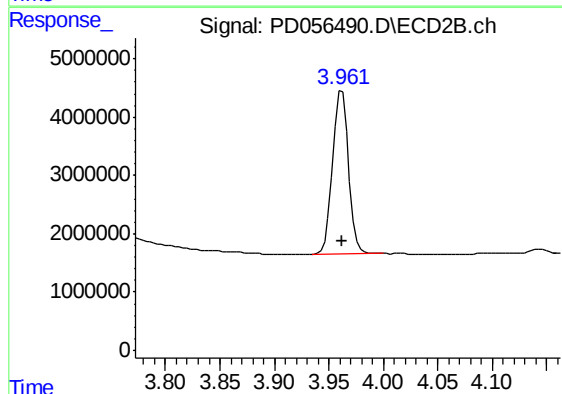


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 28462454
Conc: 23.67 ng/ml

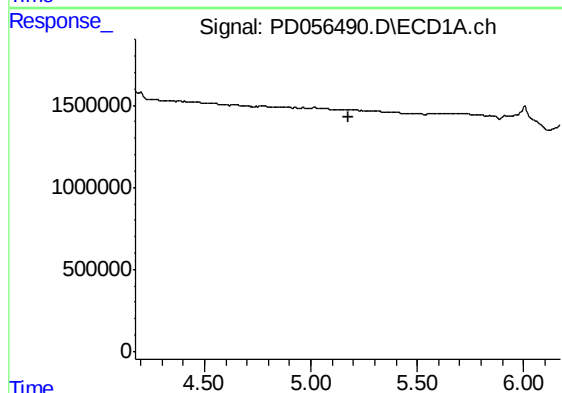


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

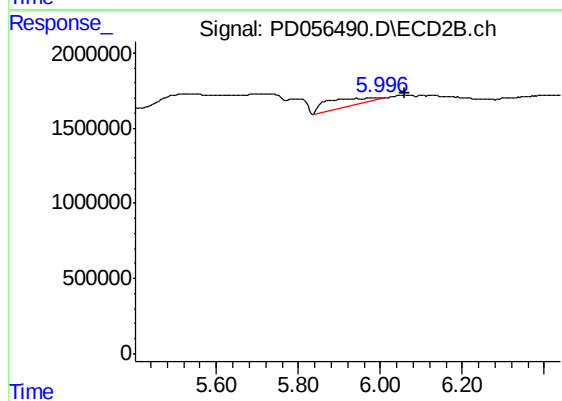

#10 trans-Chlordane


R.T.: 5.998 min
Delta R.T.: -0.062 min
Response: 3999034
Conc: 2.42 ng/ml

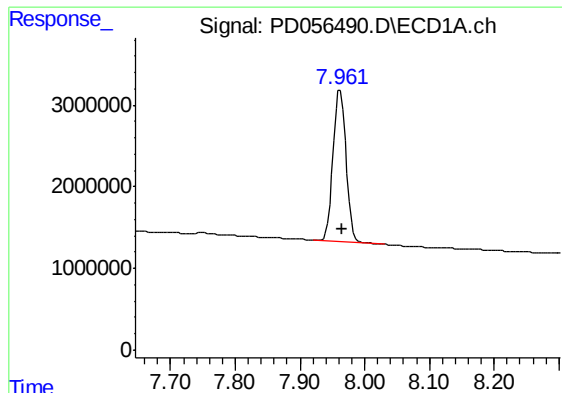

#27 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.003 min
Response: 25754789
Conc: 28.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0C09

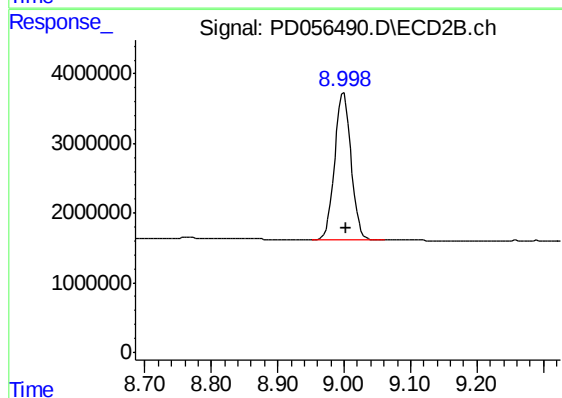

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.003 min
Response: 36383374
Conc: 30.24 ng/ml