

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
 Data File : PD056496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 13:19
 Operator : SG\AJ
 Sample : K6238-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFPZ8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:42:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.962	18193685	31222519	21.968	25.970
27)	SA Decachlor...	7.962	9.000	33082988	46095800	36.638	38.313
Target Compounds							
3)	MA gamma-BHC...	0.000	4.661f	0	754257	N.D.	0.467
4)	MA Heptachlor	0.000	5.119	0	1500936	N.D.	0.921
5)	MB Aldrin	4.530	0.000	2232669	0	2.056	N.D. #
6)	B beta-BHC	4.201f	0.000	17933121	0	33.318	N.D. #
7)	B delta-BHC	0.000	4.994	0	22919725	N.D.	13.760
10)	B trans-Chl...	0.000	6.043	0	1288475	N.D.	0.779


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
Data File : PD056496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 13:19
Operator : SG\AJ
Sample : K6238-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFPZ8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:42:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

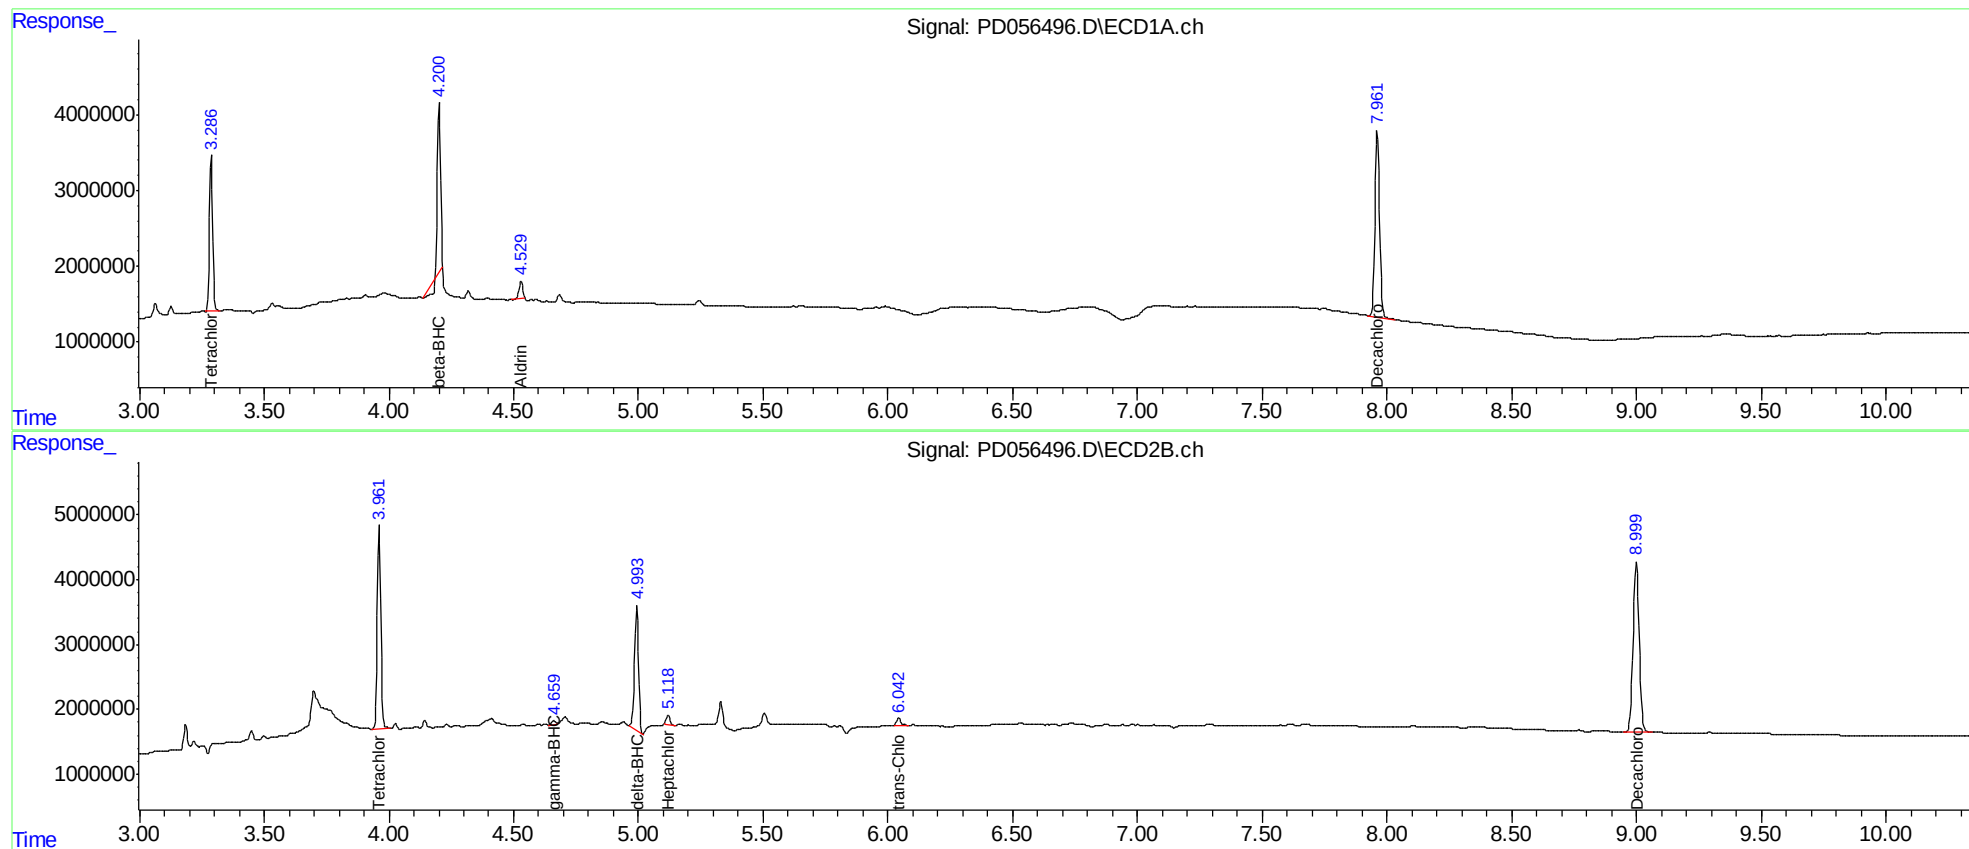


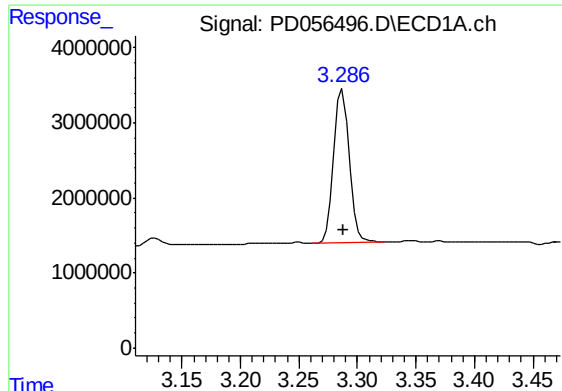

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: 0.000 min
Response: 18193685
Conc: 21.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFPZ8

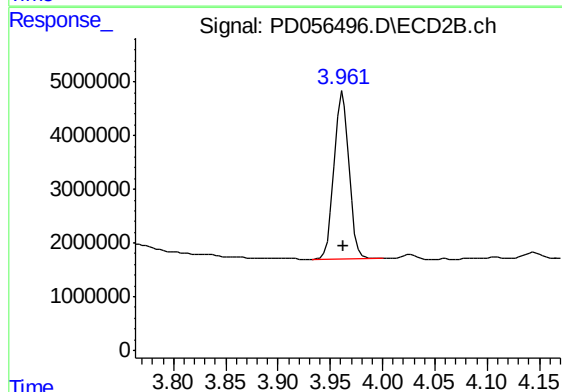


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 31222519
Conc: 25.97 ng/ml

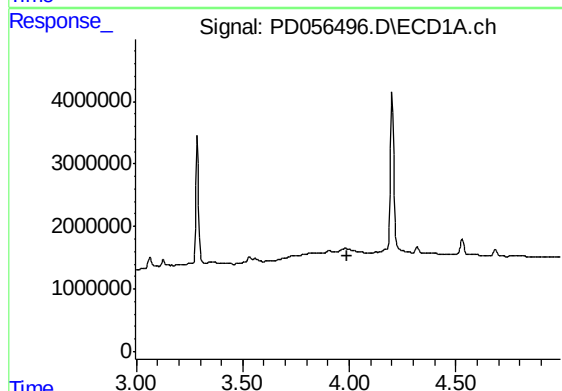


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.991 min
Response: 0
Conc: N.D.

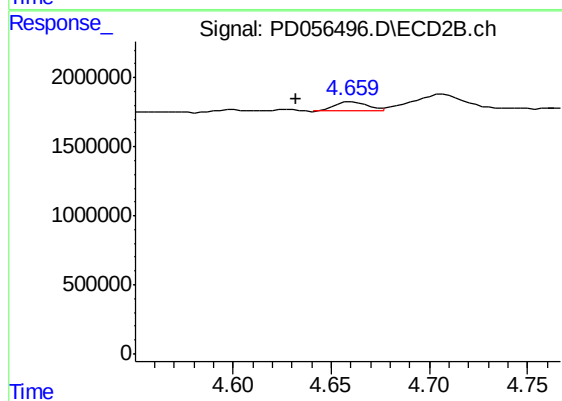

#3 gamma-BHC (Lindane)


R.T.: 4.661 min
Delta R.T.: 0.029 min
Response: 754257
Conc: 0.47 ng/ml

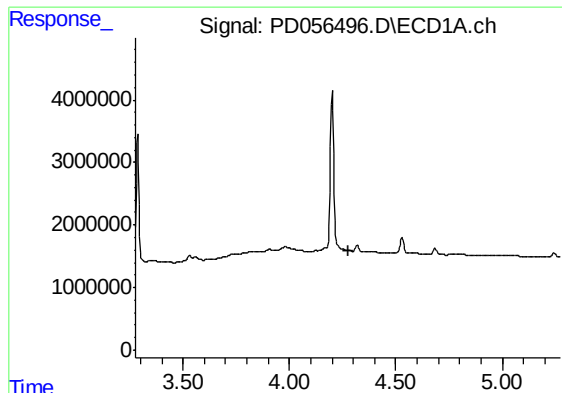

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFPZ8

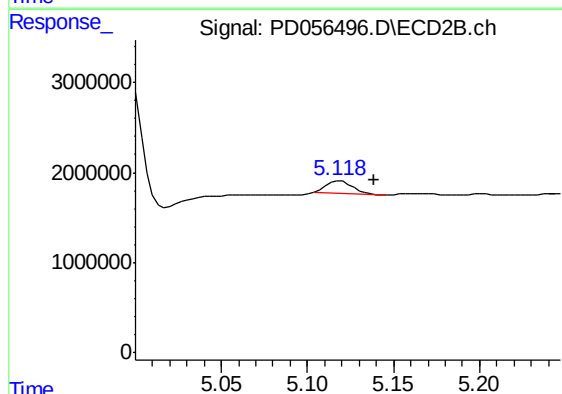


#4 Heptachlor

R.T.: 5.119 min
Delta R.T.: -0.020 min
Response: 1500936
Conc: 0.92 ng/ml

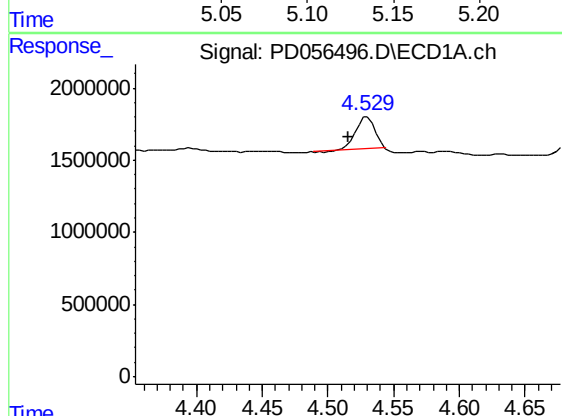


#5 Aldrin

R.T.: 4.530 min
Delta R.T.: 0.014 min
Response: 2232669
Conc: 2.06 ng/ml

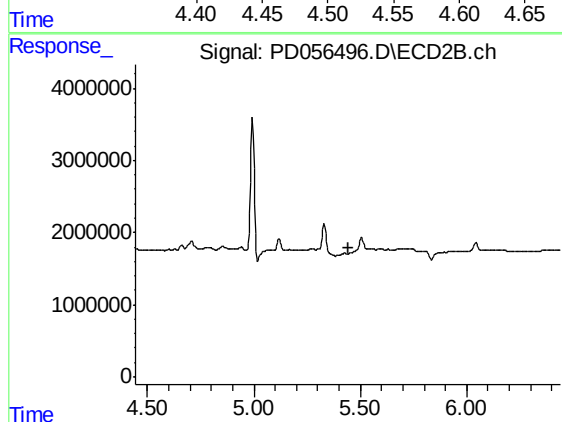

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.442 min
Response: 0
Conc: N.D.

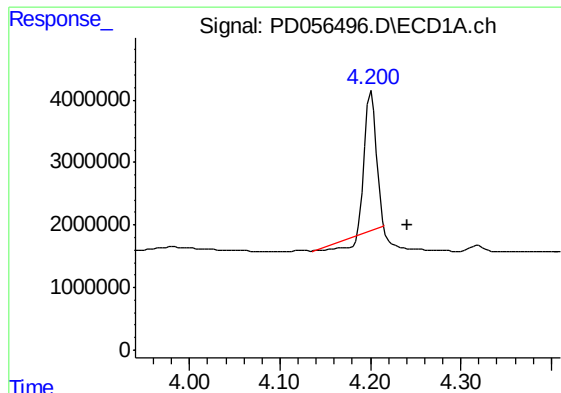

#6 beta-BHC


R.T.: 4.201 min
Delta R.T.: -0.039 min
Response: 17933121
Conc: 33.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFPZ8

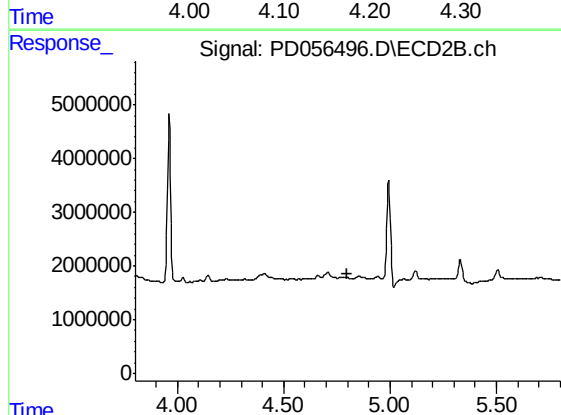


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

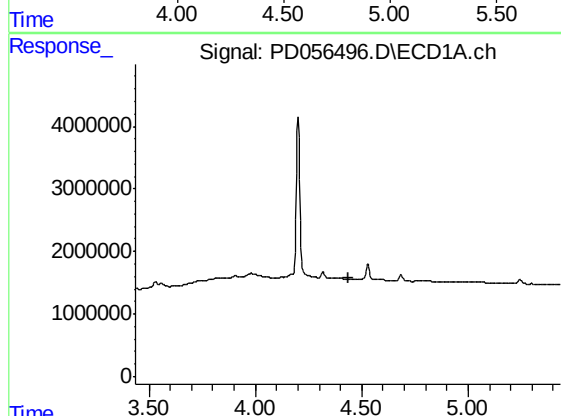


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

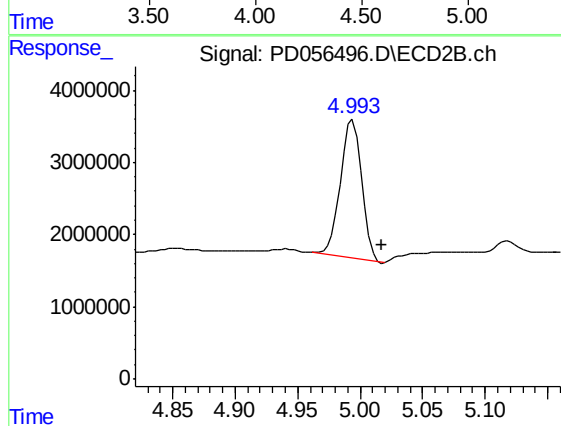

#7 delta-BHC


R.T.: 4.994 min
Delta R.T.: -0.023 min
Response: 22919725
Conc: 13.76 ng/ml

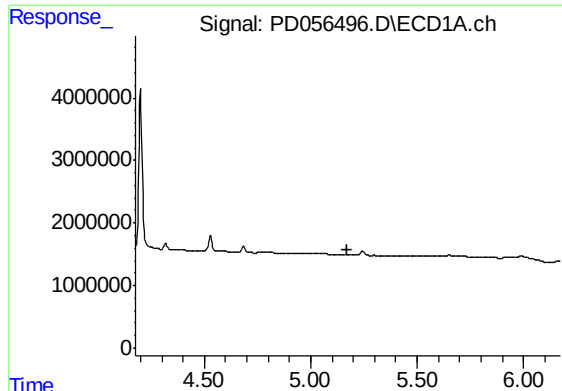

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFPZ8

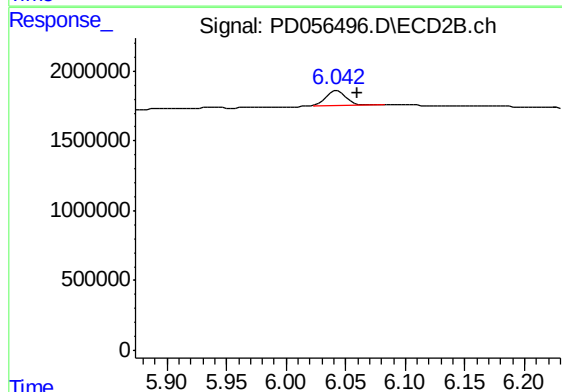


#10 trans-Chlordane

R.T.: 6.043 min
Delta R.T.: -0.017 min
Response: 1288475
Conc: 0.78 ng/ml

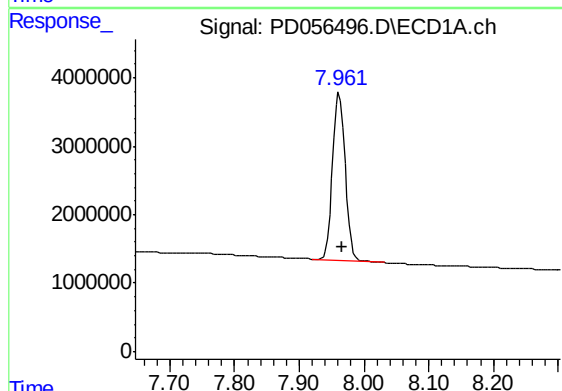

#27 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.003 min
Response: 33082988
Conc: 36.64 ng/ml

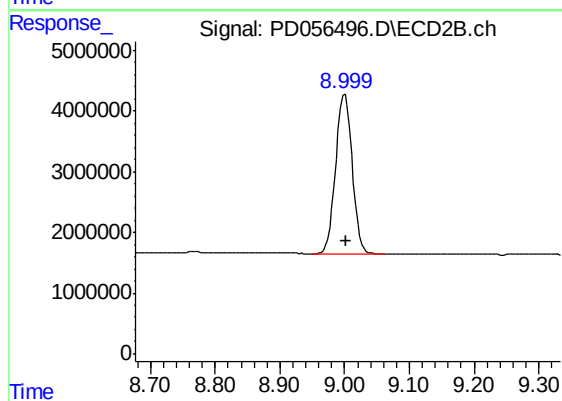

#27 Decachlorobiphenyl

R.T.: 9.000 min
Delta R.T.: -0.002 min
Response: 46095800
Conc: 38.31 ng/ml