

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
 Data File : PD056497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 13:33
 Operator : SG\AJ
 Sample : K6171-18
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BZ8

Manual Integrations
 APPROVED

Ankita
 12/18/2019 10:44:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:42:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.287	3.961	7285778	11745581	8.797	9.770
2) SA Decachlor...	7.962	8.998	12253577	17778333	13.570	14.777m
Target Compounds						
3) MA gamma-BHC...	3.995	4.612	2368306	1881356	2.109m	1.166m#
10) B trans-Chl...	5.173	6.053	1937622	8849902	1.848m	5.352m#
11) B cis-Chlor...	5.230	6.132	1565654	3372632	1.533m	2.093 #
14) MA Endrin	5.775	6.645	649816	1179891	0.778m	0.932m
16) A 4,4'-DDD	5.915	6.777	693628	1516230	0.975m	1.288 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
Data File : PD056497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 13:33
Operator : SG\AJ
Sample : K6171-18
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:42:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

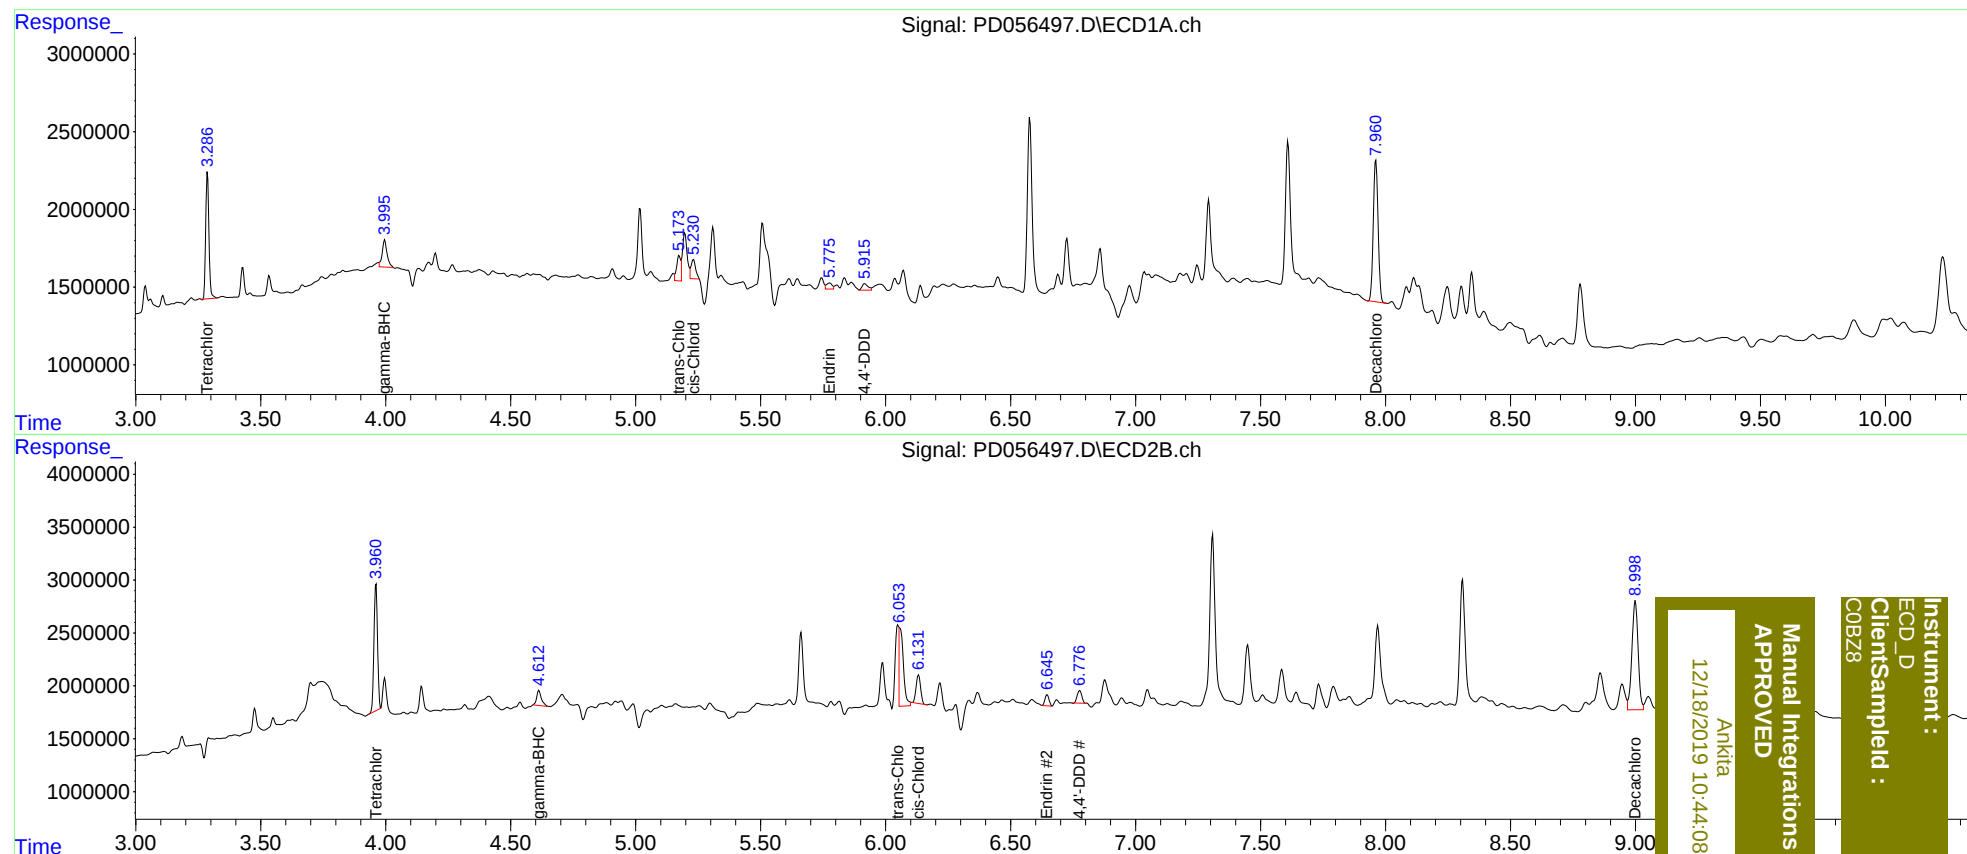

12/18/2019 10:44:08 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
C0BZ8