

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
 Data File : PD056500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2019 14:15
 Operator : SG\AJ
 Sample : K6171-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BY9

Manual Integrations
 APPROVED

Ankita
 12/18/2019 10:44:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 00:43:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.288	3.962	6476299	10695180	7.820	8.896
2) SA Decachlor...	7.962	8.999	11741485	14997802	13.003	12.465m
Target Compounds						
10) B trans-Chl...	5.172	6.048	757602	4751043	0.723m	2.873m#
11) B cis-Chlor...	5.231	6.132	887825	1307654	0.869m	0.811m
16) A 4,4'-DDD	5.914	6.778	364958	1207109	0.513m	1.026m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121719\
Data File : PD056500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2019 14:15
Operator : SG\AJ
Sample : K6171-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 00:43:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

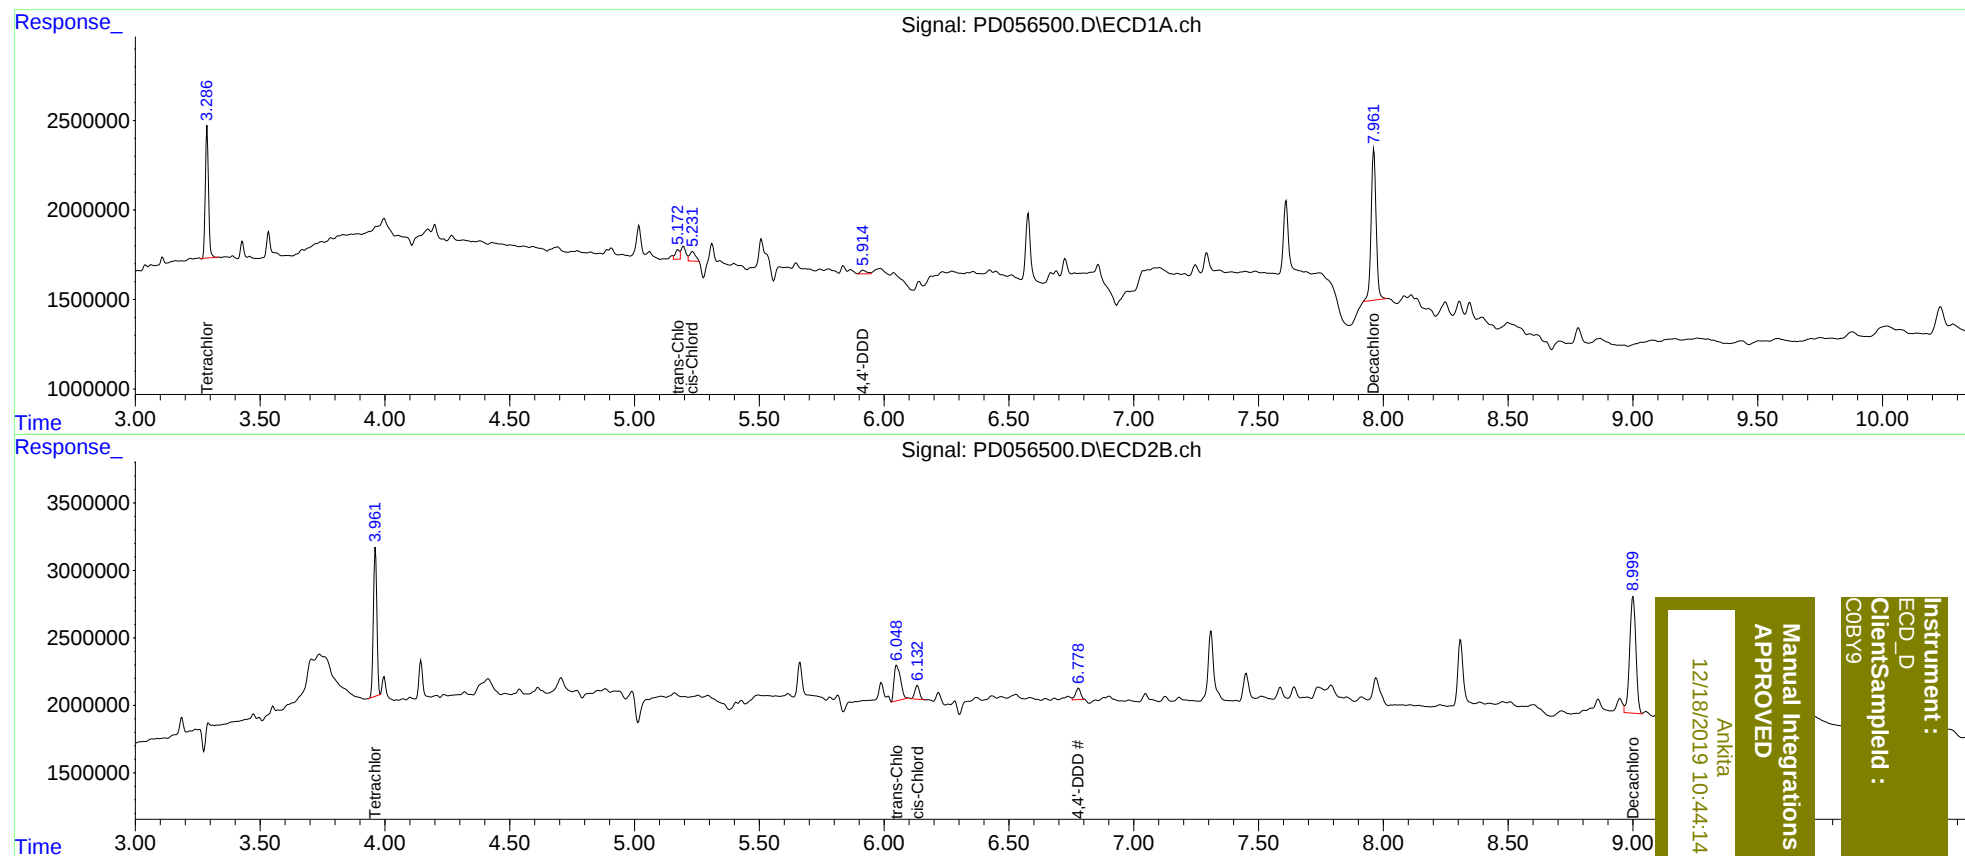

12/18/2019 10:44:14 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
C0BY9