

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121720\
 Data File : PD060761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 11:59
 Operator : DD\AJ
 Sample : L5091-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 12:42:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 03:53:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.501	4.022	14094673	61212272	12.964	13.025
28)	SA Decachlor...	8.288	9.108	17155392	48732824	12.144	13.044
Target Compounds							
8)	B Heptachlo...	0.000	5.892	0	1612493	N.D.	0.289 #
10)	B gamma-Chl...	0.000	6.150	0	3013684	N.D.	0.522 #
12)	B 4,4'-DDE	5.682	6.365	1072005	7691737	0.718	1.454 #
14)	MA Endrin	0.000	6.727	0	3124594	N.D.	0.665 #
16)	A 4,4'-DDD	0.000	6.862	0	3238752	N.D.	0.736 #
17)	MA 4,4'-DDT	6.440	7.156	1856716	2439345	1.411	0.547 #
20)	A Methoxychlor	6.976	0.000	1295548	0	1.664	N.D. #
25)	Chlordane-3	0.000	6.150	0	3013684	N.D.	4.245 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121720\
Data File : PD060761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 11:59
Operator : DD\AJ
Sample : L5091-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 12:42:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 03:53:08 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

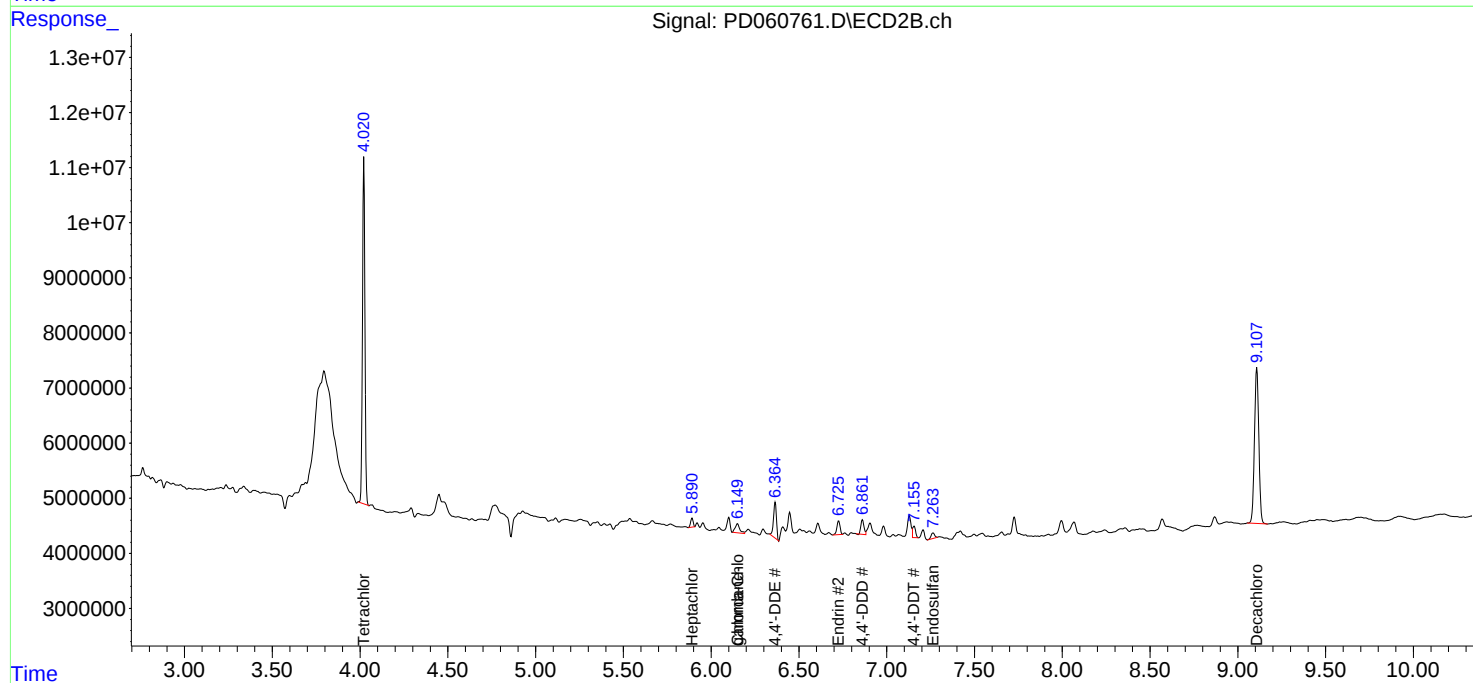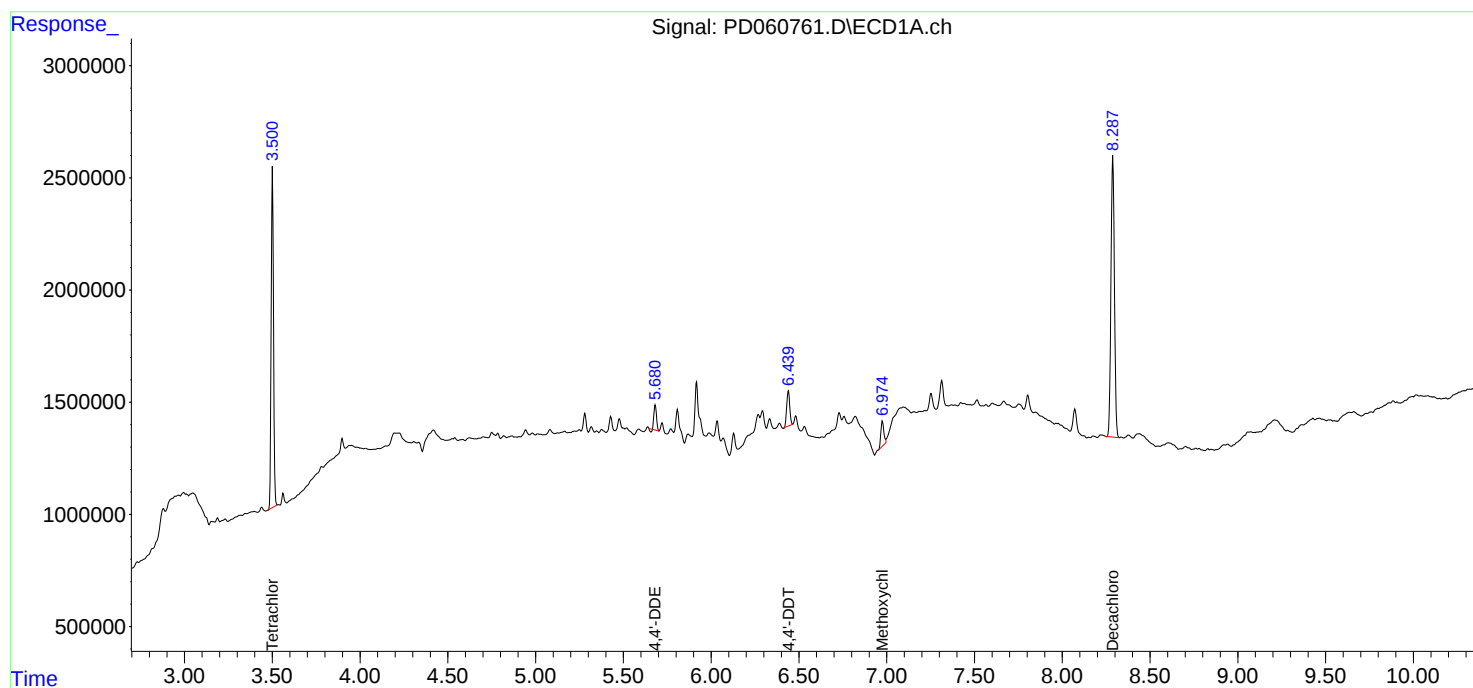


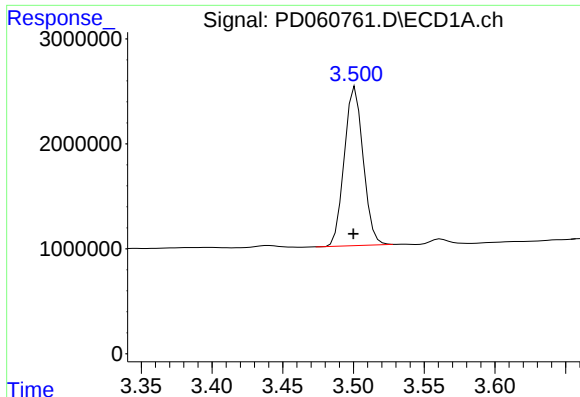

#1 Tetrachloro-m-xylene


R.T.: 3.501 min
Delta R.T.: 0.001 min
Response: 14094673
Conc: 12.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

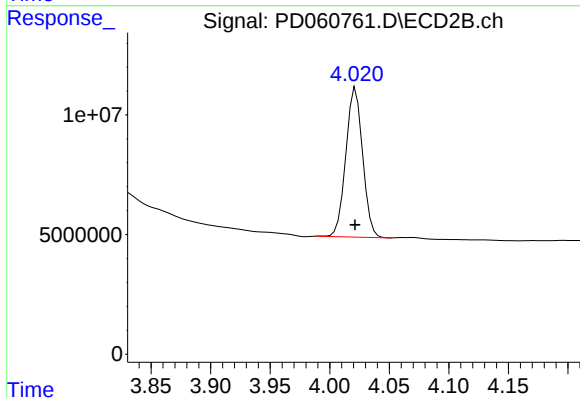


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 61212272
Conc: 13.03 ng/ml

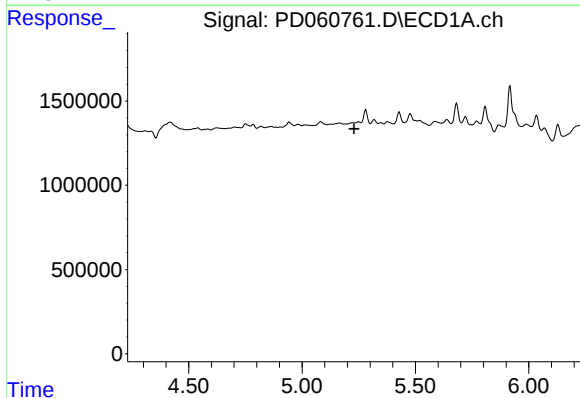


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.229 min
Response: 0
Conc: N.D.

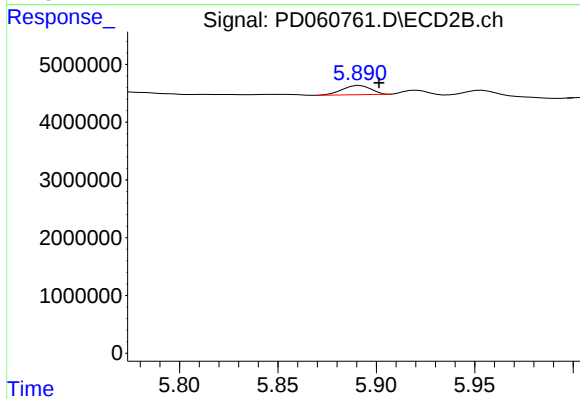

#8 Heptachlor epoxide


R.T.: 5.892 min
Delta R.T.: -0.010 min
Response: 1612493
Conc: 0.29 ng/ml

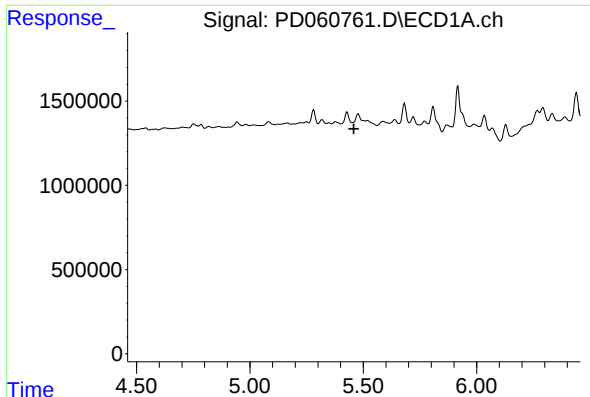

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

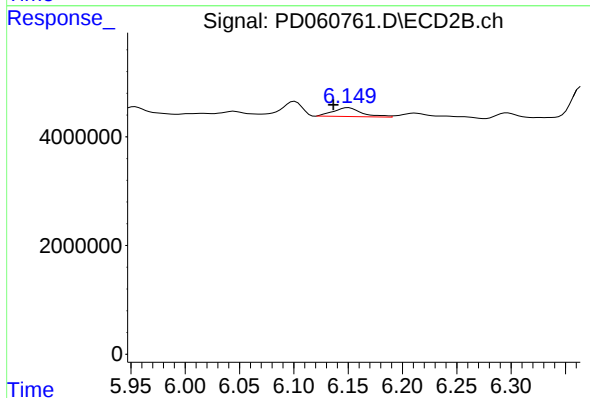


#10 gamma-Chlordane

R.T.: 6.150 min
Delta R.T.: 0.014 min
Response: 3013684
Conc: 0.52 ng/ml

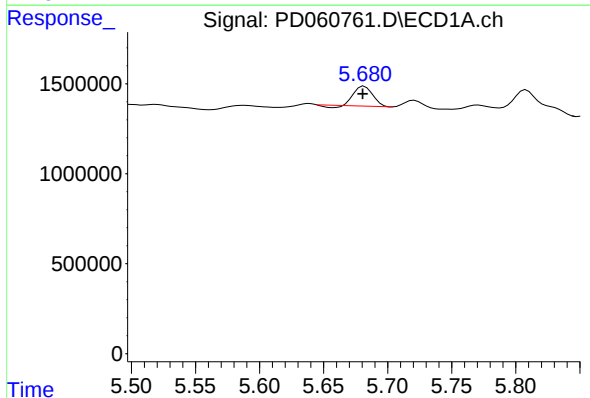


#12 4,4'-DDE

R.T.: 5.682 min
Delta R.T.: 0.001 min
Response: 1072005
Conc: 0.72 ng/ml

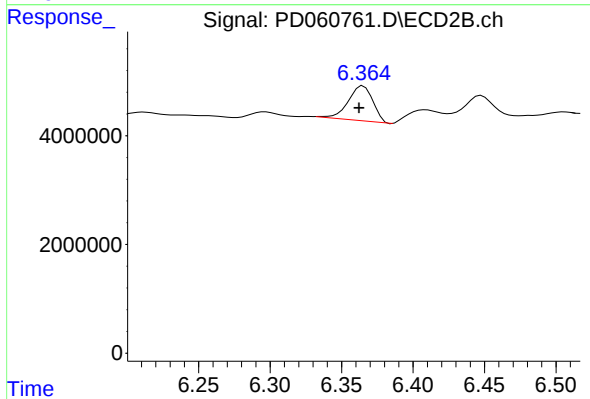

#12 4,4'-DDE


R.T.: 6.365 min
Delta R.T.: 0.003 min
Response: 7691737
Conc: 1.45 ng/ml

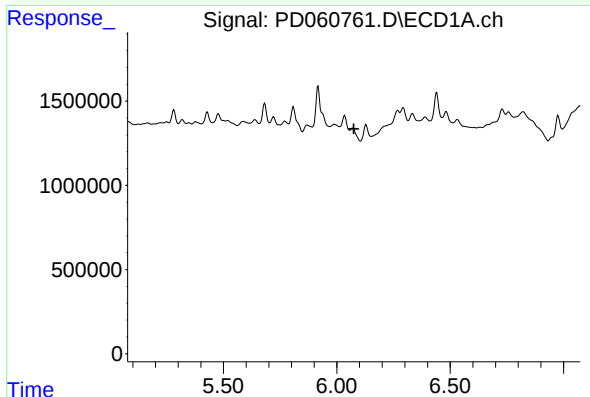

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

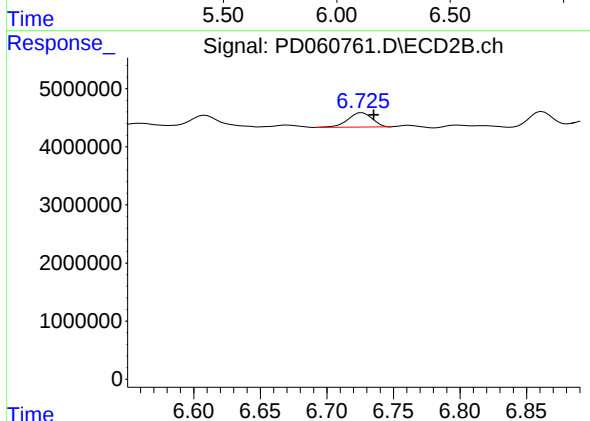


#14 Endrin

R.T.: 6.727 min
Delta R.T.: -0.009 min
Response: 3124594
Conc: 0.67 ng/ml

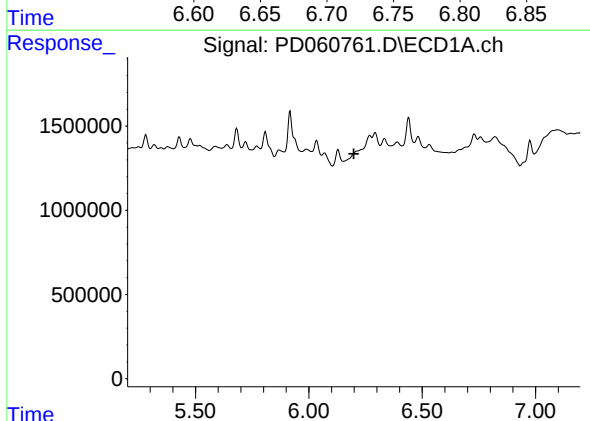


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.199 min
Response: 0
Conc: N.D.

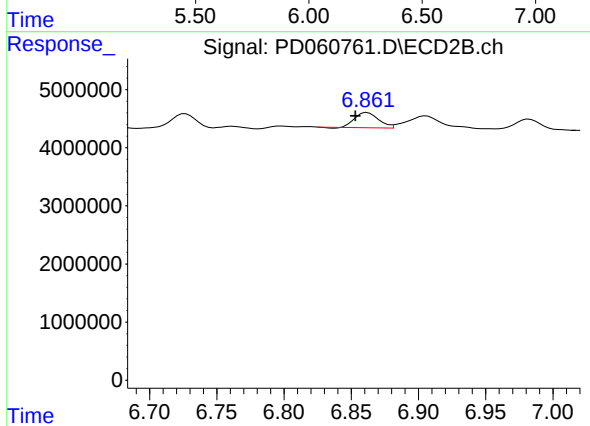

#16 4,4'-DDD


R.T.: 6.862 min
Delta R.T.: 0.009 min
Response: 3238752
Conc: 0.74 ng/ml

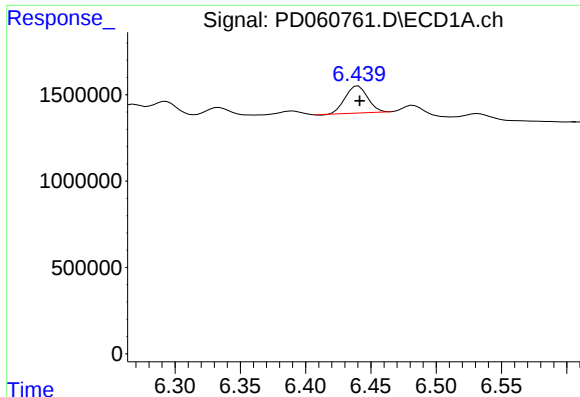

#17 4,4'-DDT


R.T.: 6.440 min
Delta R.T.: -0.001 min
Response: 1856716
Conc: 1.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

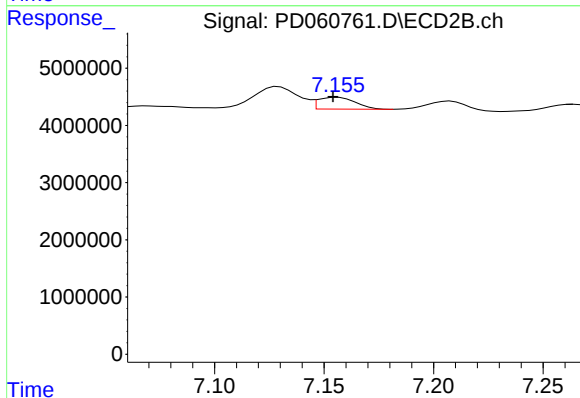


#17 4,4'-DDT

R.T.: 7.156 min
Delta R.T.: 0.002 min
Response: 2439345
Conc: 0.55 ng/ml

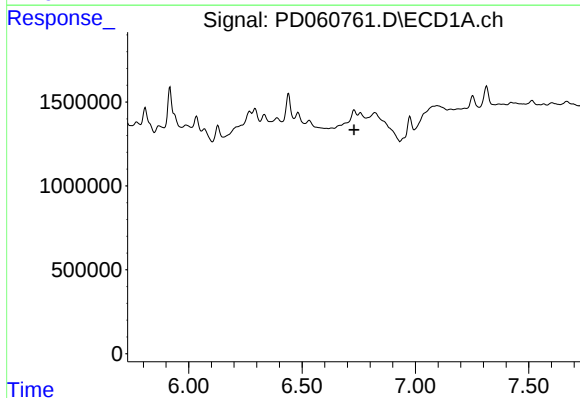


#19 Endosulfan Sulfate

R.T.: 6.730 min
Delta R.T.: 0.000 min
Response: -559008
Conc: N.D.

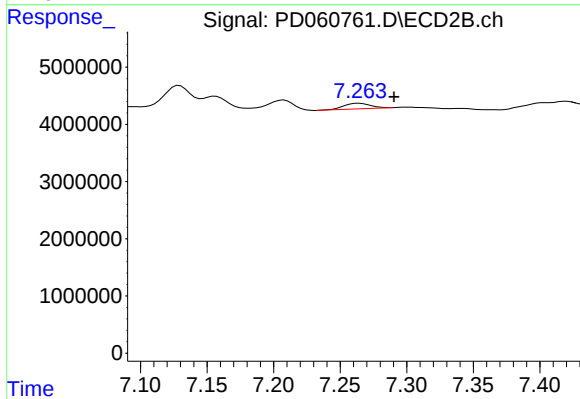

#19 Endosulfan Sulfate


R.T.: 7.264 min
Delta R.T.: -0.026 min
Response: 1355255
Conc: 0.31 ng/ml

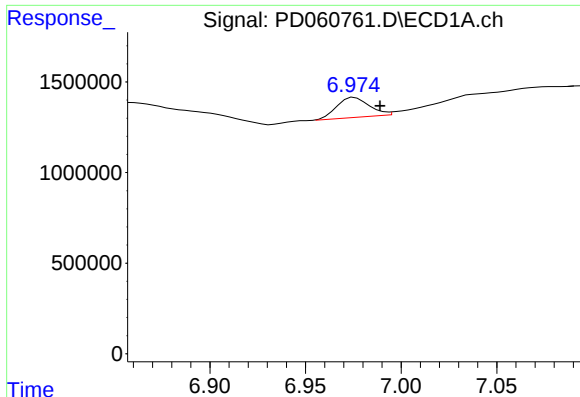

#20 Methoxychlor


R.T.: 6.976 min
Delta R.T.: -0.013 min
Response: 1295548
Conc: 1.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

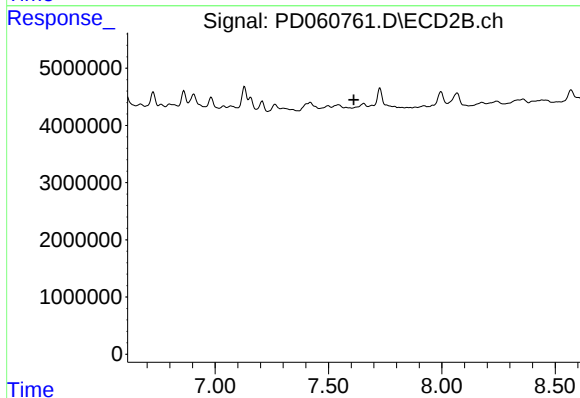


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.611 min
Response: 0
Conc: N.D.

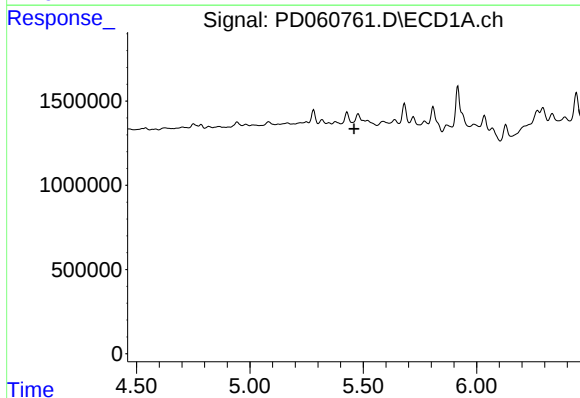


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.459 min
Response: 0
Conc: N.D.

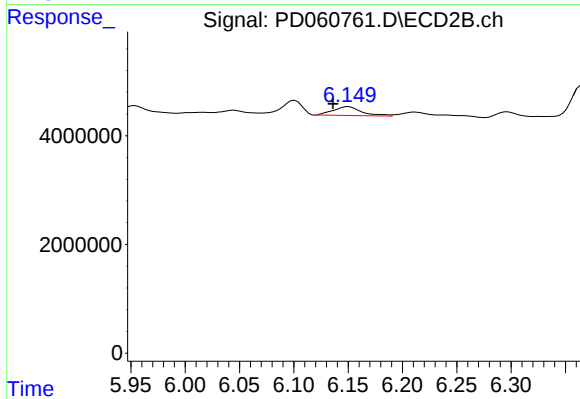

#25 Chlordane-3


R.T.: 6.150 min
Delta R.T.: 0.014 min
Response: 3013684
Conc: 4.24 ng/ml

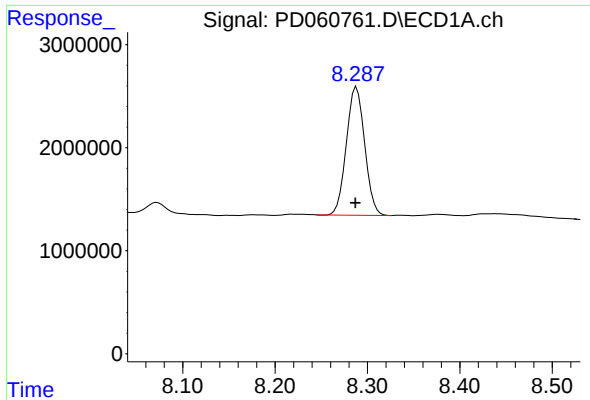

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: 0.001 min
Response: 17155392
Conc: 12.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

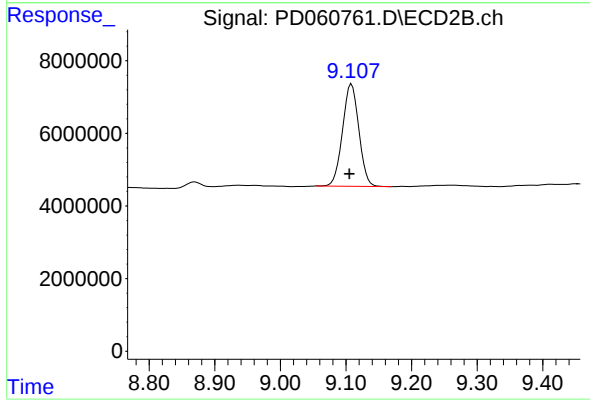

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: 0.003 min
Response: 48732824
Conc: 13.04 ng/ml