

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121720\
 Data File : PD060762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 12:13
 Operator : DD\AJ
 Sample : L5091-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 12:42:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 03:53:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.501	4.022	14147567	60079309	13.012	12.784
28)	SA Decachlor...	8.290	9.108	16913521	46578730	11.973	12.467
Target Compounds							
5)	MB Aldrin	0.000	5.538f	0	2055387	N.D.	0.337 #
8)	B Heptachlo...	0.000	5.892	0	2869250	N.D.	0.513 #
10)	B gamma-Chl...	0.000	6.151	0	4393452	N.D.	0.761 #
12)	B 4,4'-DDE	5.682	6.366	12356502	47744812	8.274	9.026
14)	MA Endrin	0.000	6.727	0	3036837	N.D.	0.647 #
16)	A 4,4'-DDD	0.000	6.862	0	3562912	N.D.	0.810 #
17)	MA 4,4'-DDT	6.441	7.156	3070687	6060893	2.333	1.359 #
20)	A Methoxychlor	6.975	0.000	1314615	0	1.688	N.D. #
25)	Chlordane-3	0.000	6.151f	0	4393452	N.D.	6.188 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121720\
Data File : PD060762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 12:13
Operator : DD\AJ
Sample : L5091-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 12:42:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 03:53:08 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

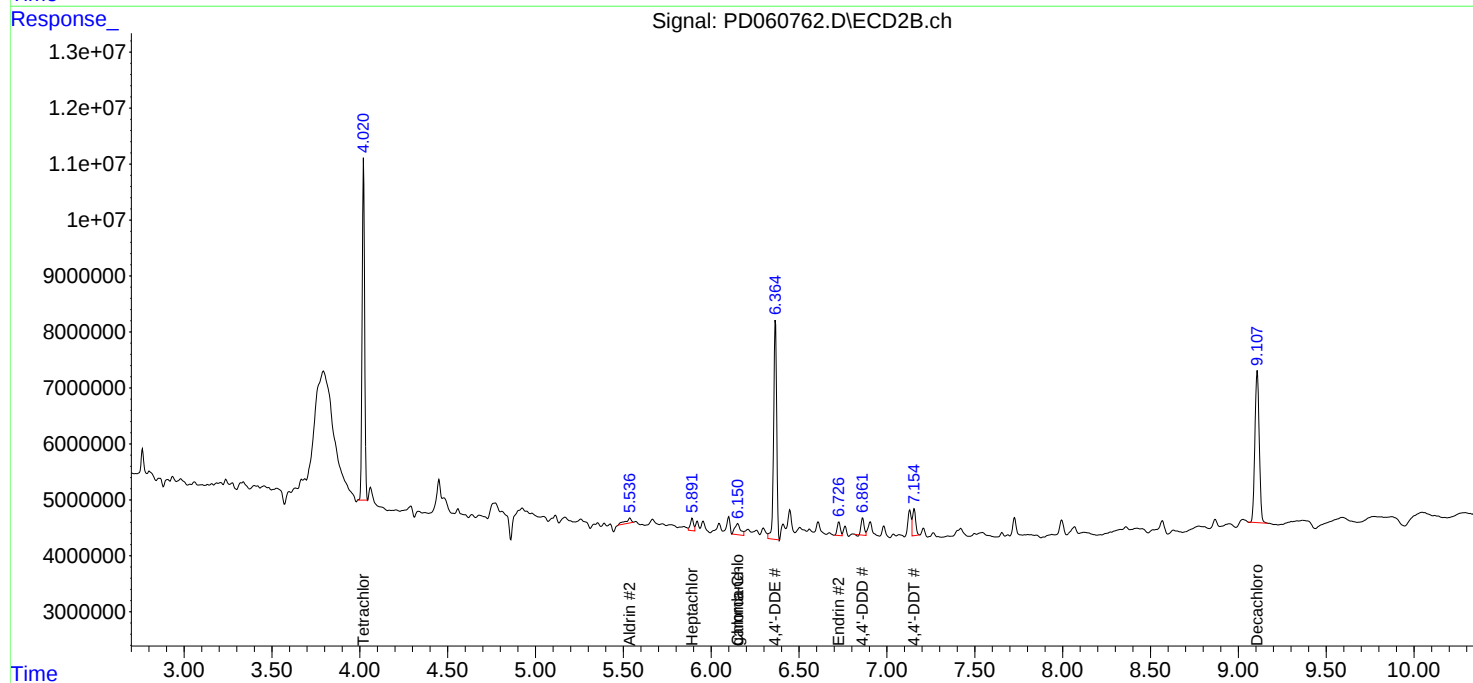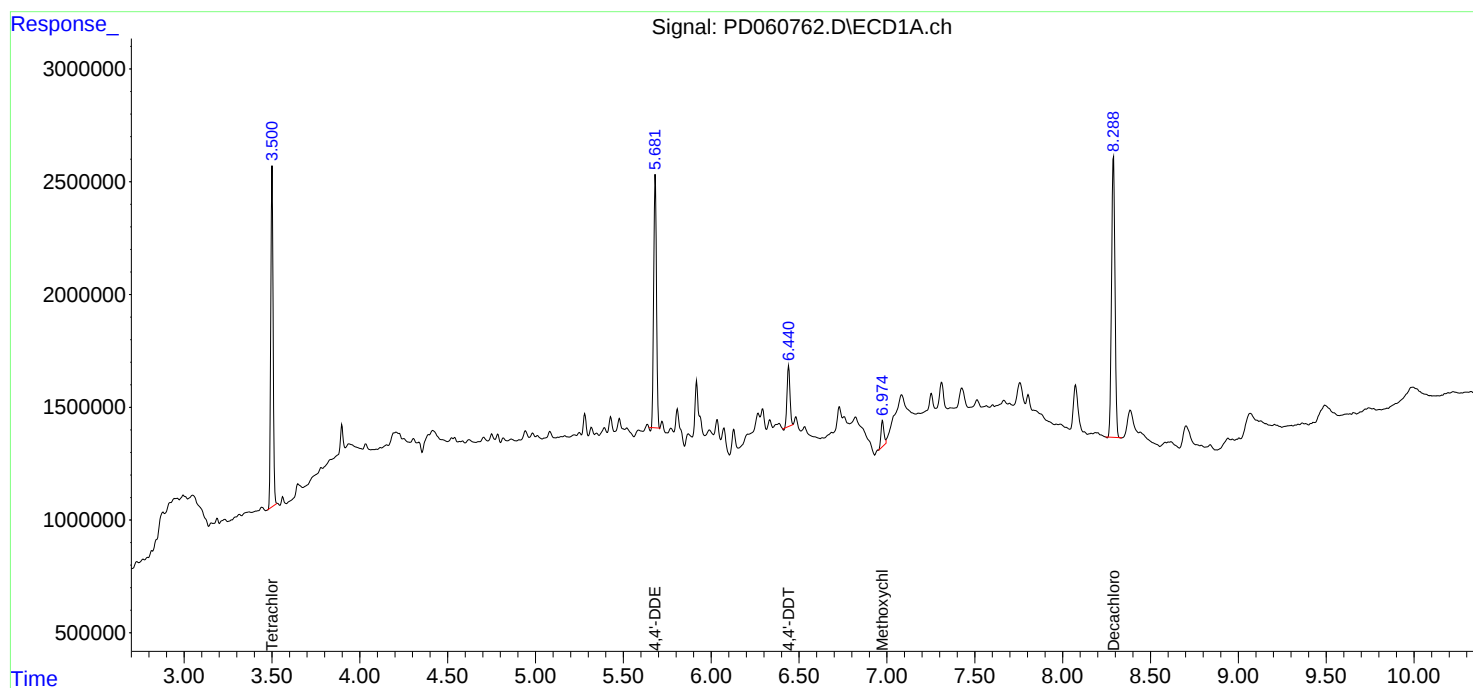


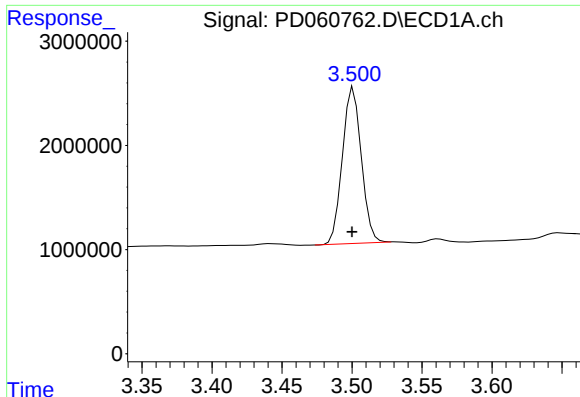

#1 Tetrachloro-m-xylene


R.T.: 3.501 min
Delta R.T.: 0.001 min
Response: 14147567
Conc: 13.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

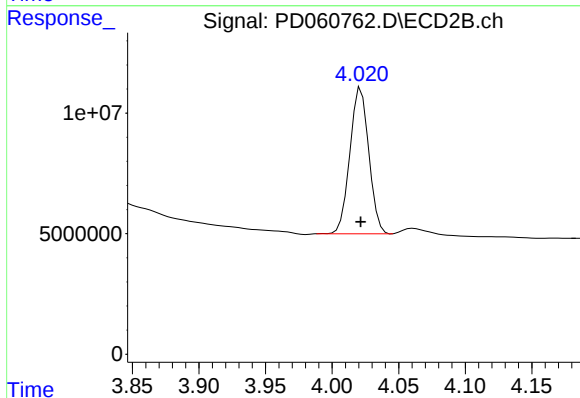


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 60079309
Conc: 12.78 ng/ml

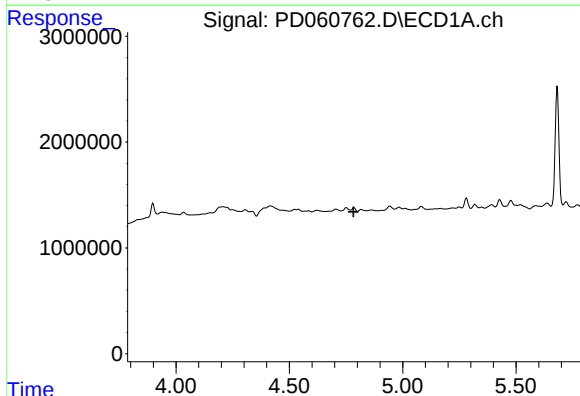


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.784 min
Response: 0
Conc: N.D.

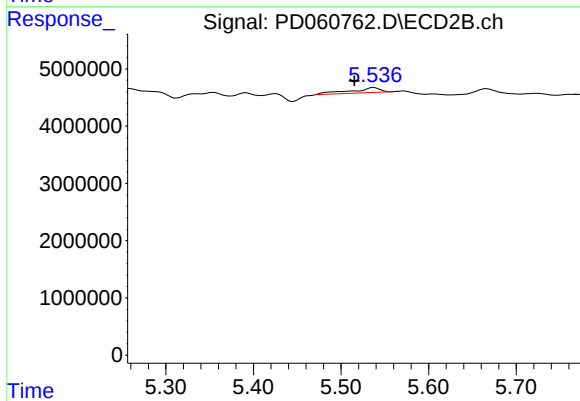

#5 Aldrin


R.T.: 5.538 min
Delta R.T.: 0.022 min
Response: 2055387
Conc: 0.34 ng/ml

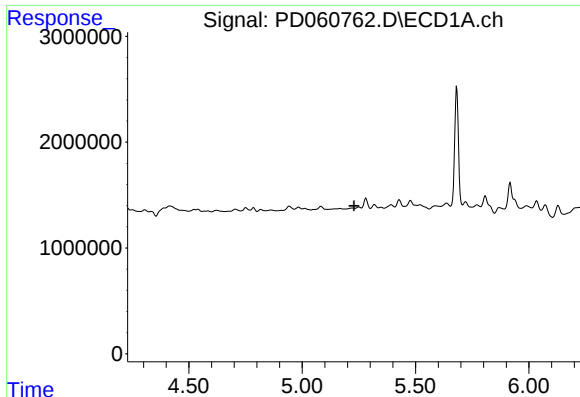

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

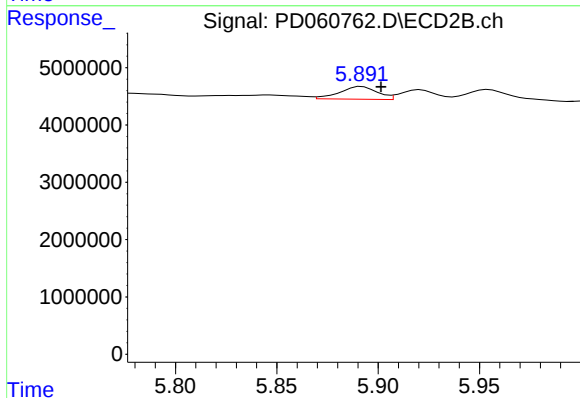


#8 Heptachlor epoxide

R.T.: 5.892 min
Delta R.T.: -0.009 min
Response: 2869250
Conc: 0.51 ng/ml

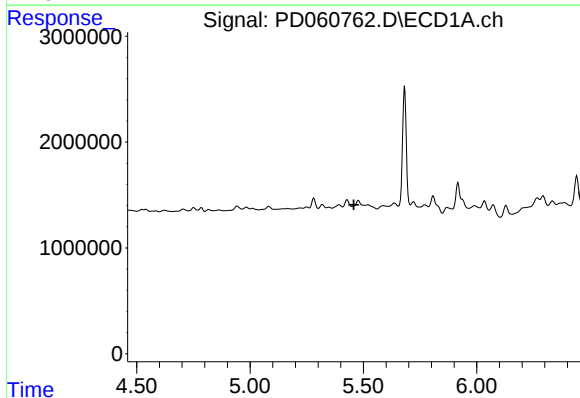


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.458 min
Response: 0
Conc: N.D.

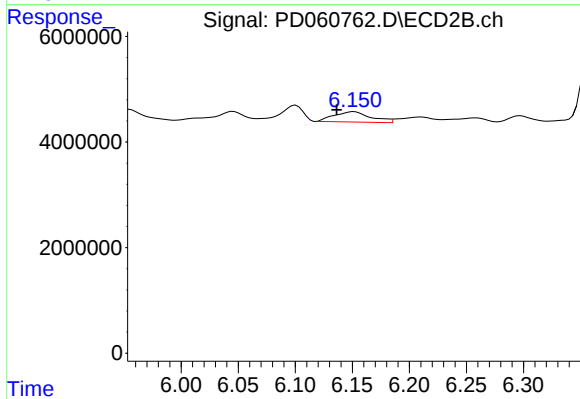

#10 gamma-Chlordane


R.T.: 6.151 min
Delta R.T.: 0.015 min
Response: 4393452
Conc: 0.76 ng/ml

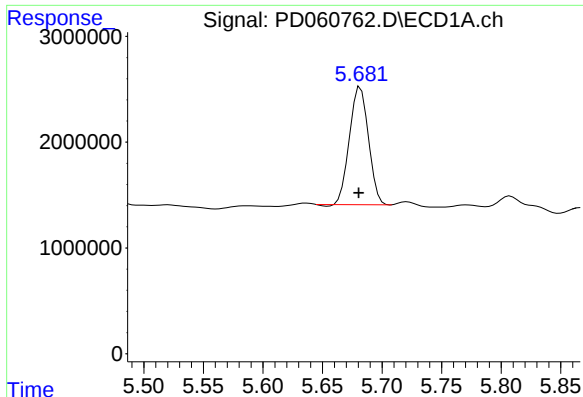

#12 4,4'-DDE


R.T.: 5.682 min
Delta R.T.: 0.001 min
Response: 12356502
Conc: 8.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

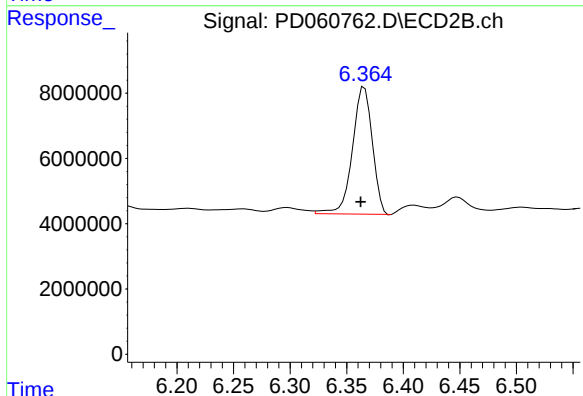


#12 4,4'-DDE

R.T.: 6.366 min
Delta R.T.: 0.003 min
Response: 47744812
Conc: 9.03 ng/ml

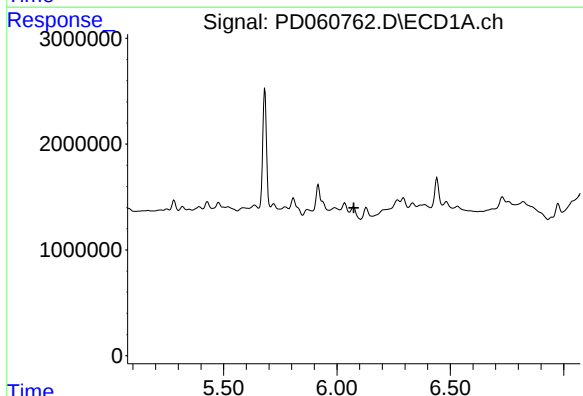


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.075 min
Response: 0
Conc: N.D.

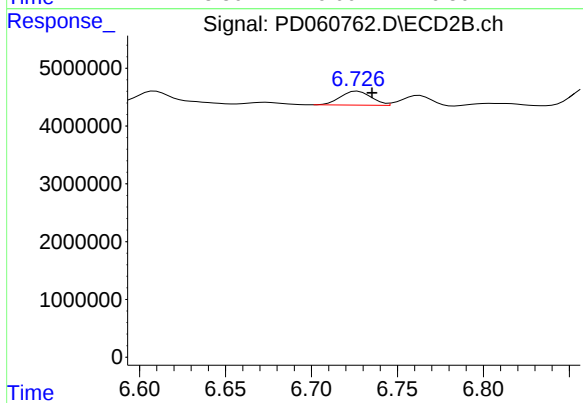

#14 Endrin


R.T.: 6.727 min
Delta R.T.: -0.008 min
Response: 3036837
Conc: 0.65 ng/ml

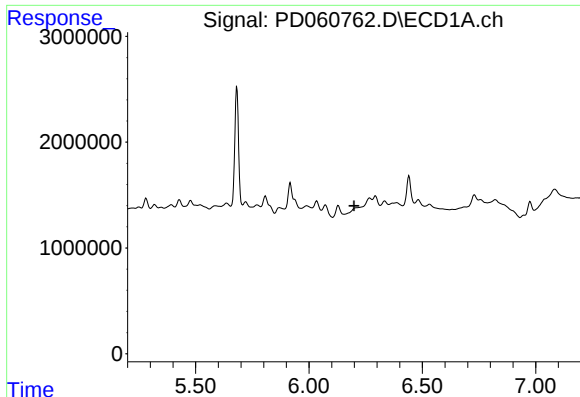

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

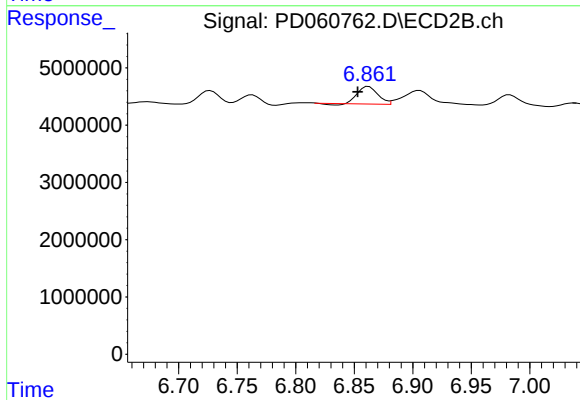


#16 4,4'-DDD

R.T.: 6.862 min
Delta R.T.: 0.009 min
Response: 3562912
Conc: 0.81 ng/ml

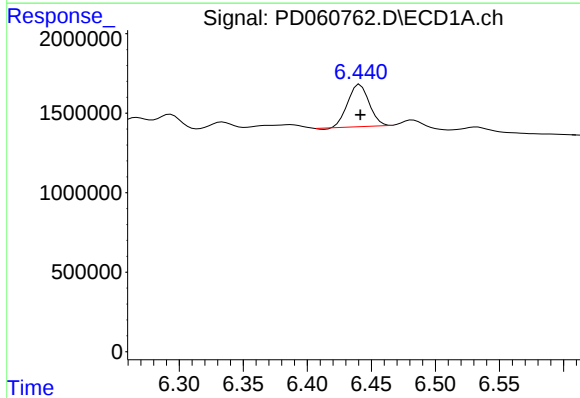


#17 4,4'-DDT

R.T.: 6.441 min
Delta R.T.: 0.000 min
Response: 3070687
Conc: 2.33 ng/ml

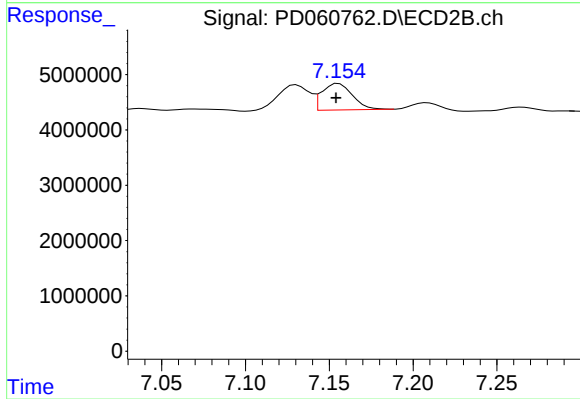

#17 4,4'-DDT


R.T.: 7.156 min
Delta R.T.: 0.002 min
Response: 6060893
Conc: 1.36 ng/ml

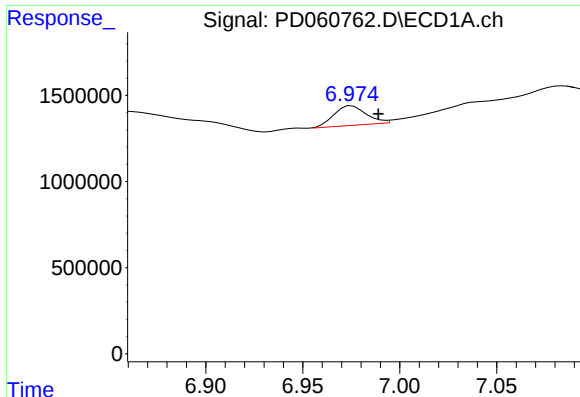

#20 Methoxychlor


R.T.: 6.975 min
Delta R.T.: -0.014 min
Response: 1314615
Conc: 1.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

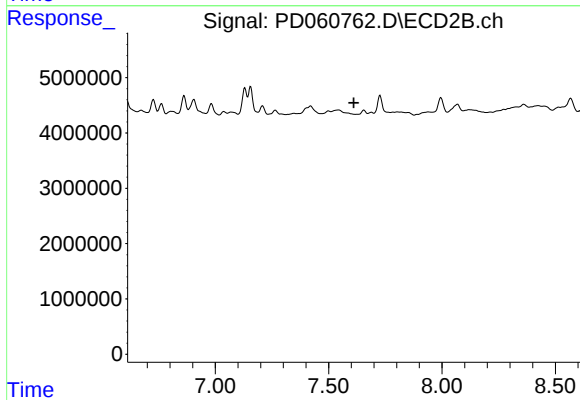


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.611 min
Response: 0
Conc: N.D.

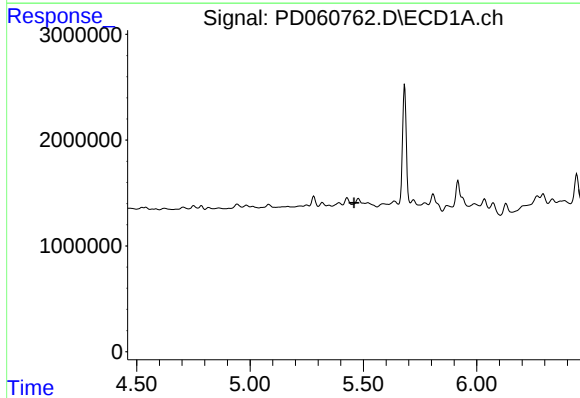


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.459 min
Response: 0
Conc: N.D.

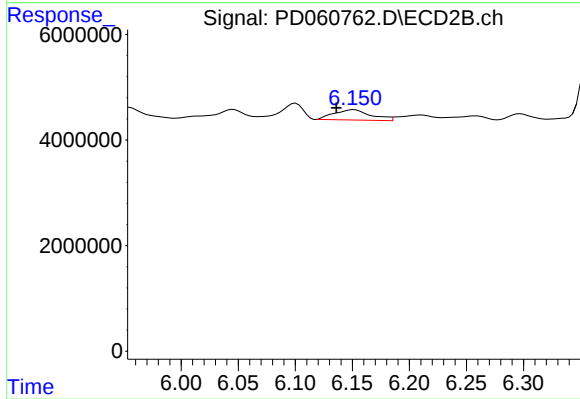

#25 Chlordane-3


R.T.: 6.151 min
Delta R.T.: 0.015 min
Response: 4393452
Conc: 6.19 ng/ml

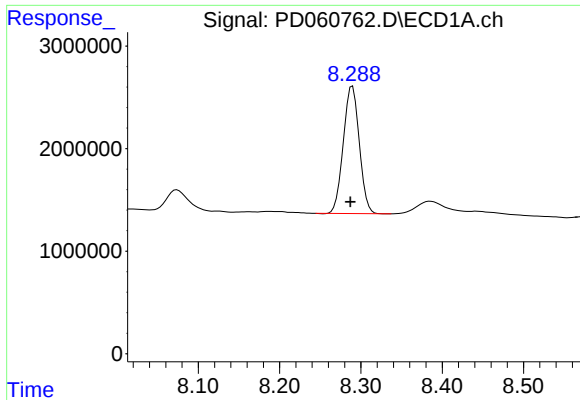

#28 Decachlorobiphenyl

R.T.: 8.290 min
Delta R.T.: 0.003 min
Response: 16913521
Conc: 11.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

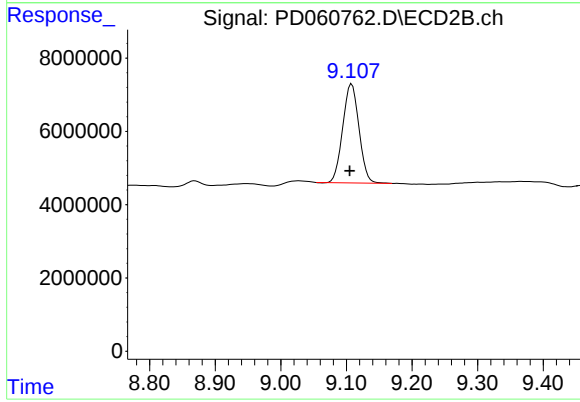

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: 0.003 min
Response: 46578730
Conc: 12.47 ng/ml