

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121720\
 Data File : PD060765.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 12:55
 Operator : DD\AJ
 Sample : L5088-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 03:03:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 03:53:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.501	4.022	13243588	55535457	12.181	11.817
28)	SA Decachlor...	8.288	9.107	18303552	47780350	12.956	12.789
Target Compounds							
8)	B Heptachlo...	0.000	5.892	0	1239568	N.D.	0.222 #
10)	B gamma-Chl...	0.000	6.139	0	2456018	N.D.	0.425 #
11)	B alpha-Chl...	0.000	6.212	0	2937681	N.D.	0.523 #
13)	MA Dieldrin	0.000	6.508	0	2211117	N.D.	0.396 #
16)	A 4,4'-DDD	0.000	6.863	0	3020170	N.D.	0.687 #
17)	MA 4,4'-DDT	6.438	7.129f	1409903	6860775	1.071	1.539 #
19)	B Endosulfa...	6.729	7.265f	-171440	2038049	N.D.	0.460
20)	A Methoxychlor	6.975	0.000	2806568	0	3.604	N.D. #
25)	Chlordane-3	0.000	6.139	0	2456018	N.D.	3.459 #
26)	Chlordane-4	0.000	6.212	0	2937681	N.D.	3.545 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121720\
Data File : PD060765.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 12:55
Operator : DD\AJ
Sample : L5088-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 03:03:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 03:53:08 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

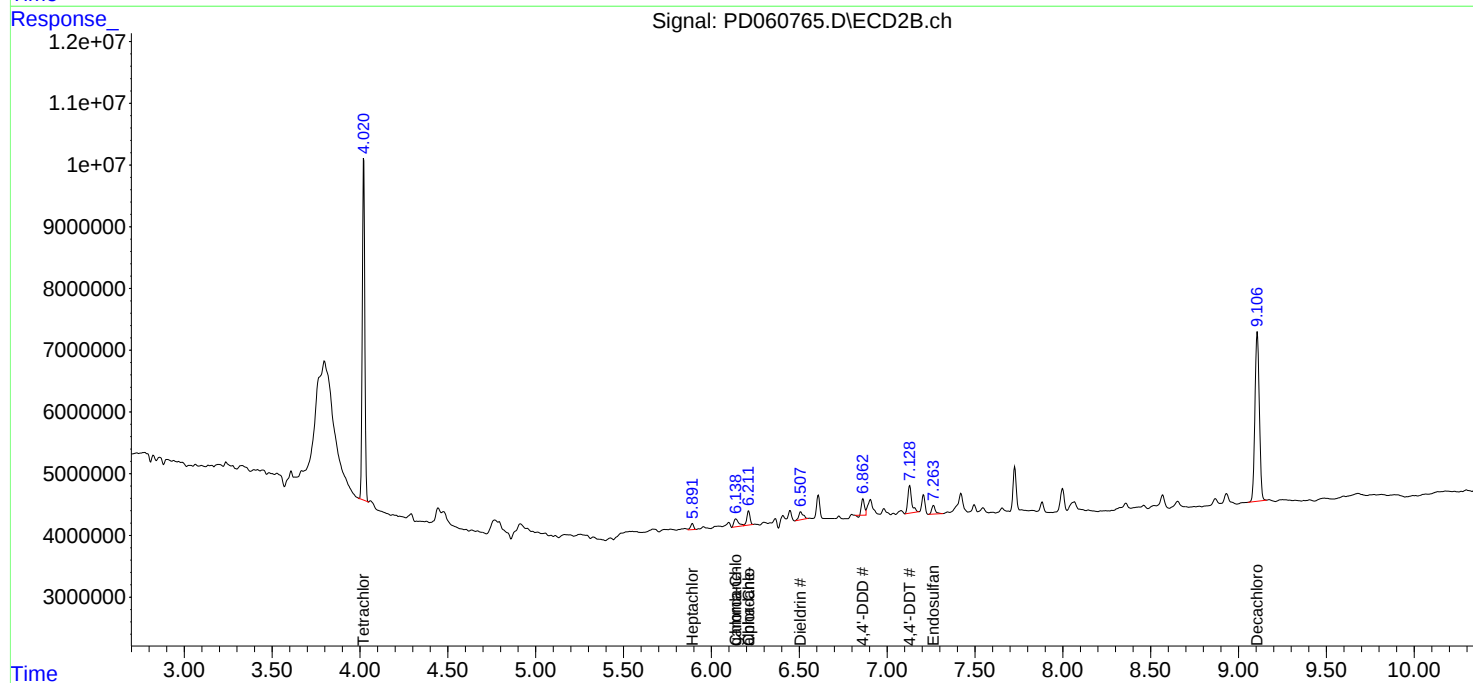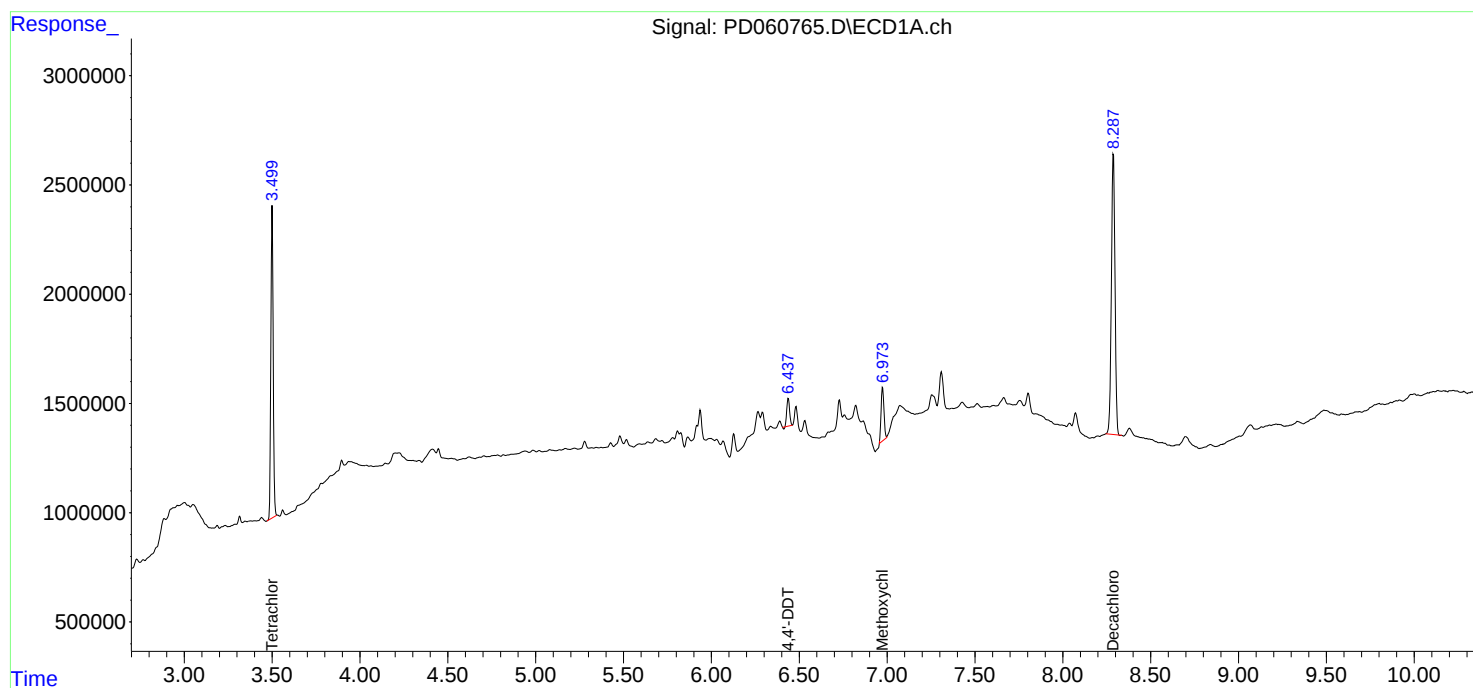


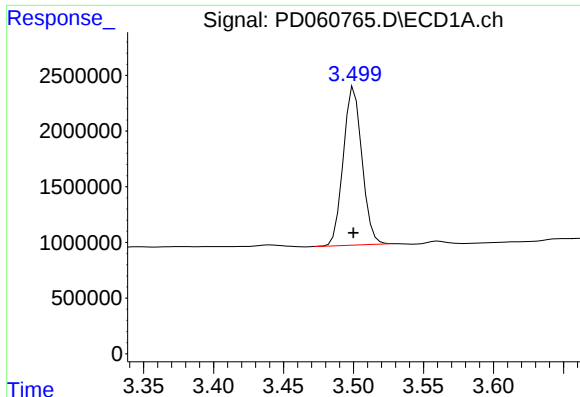

#1 Tetrachloro-m-xylene


R.T.: 3.501 min
Delta R.T.: 0.000 min
Response: 13243588
Conc: 12.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

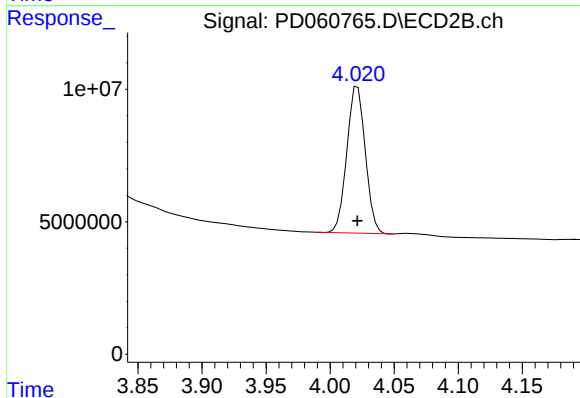


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 55535457
Conc: 11.82 ng/ml

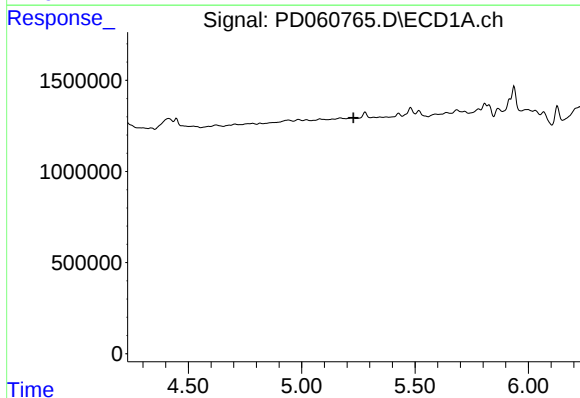


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.229 min
Response: 0
Conc: N.D.

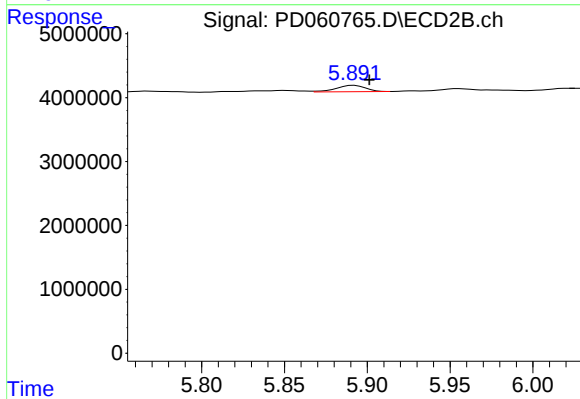

#8 Heptachlor epoxide


R.T.: 5.892 min
Delta R.T.: -0.009 min
Response: 1239568
Conc: 0.22 ng/ml

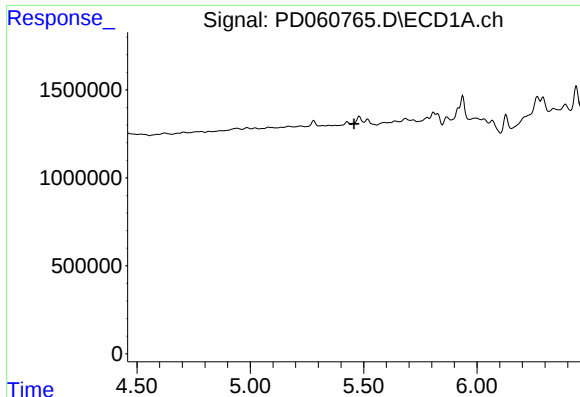

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

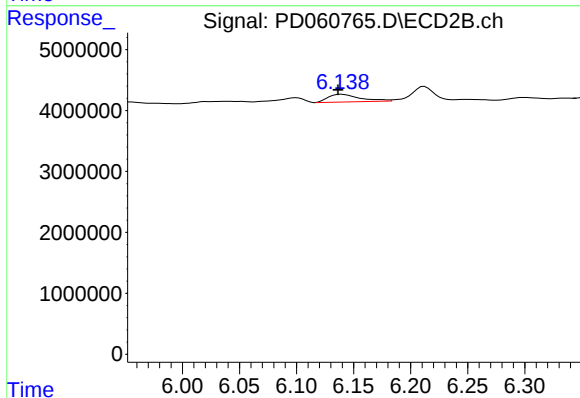


#10 gamma-Chlordane

R.T.: 6.139 min
Delta R.T.: 0.003 min
Response: 2456018
Conc: 0.43 ng/ml

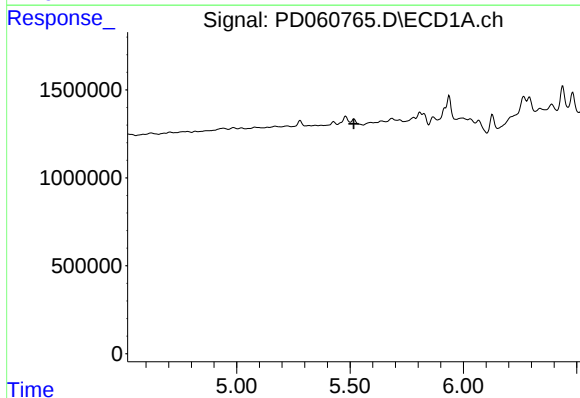


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.517 min
Response: 0
Conc: N.D.

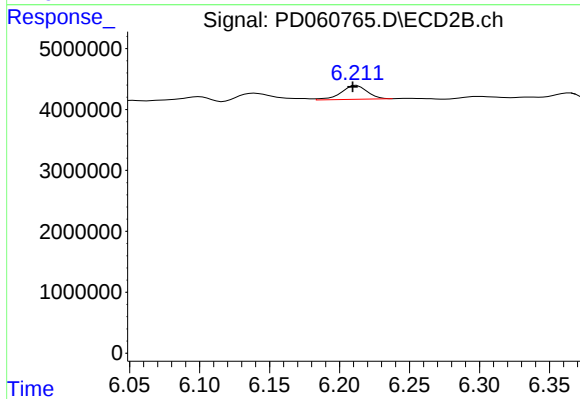

#11 alpha-Chlordane


R.T.: 6.212 min
Delta R.T.: 0.003 min
Response: 2937681
Conc: 0.52 ng/ml

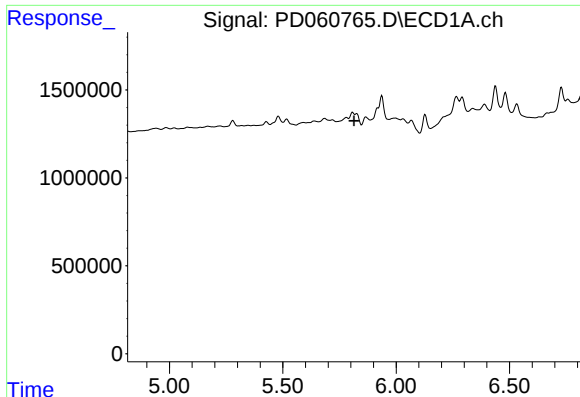

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

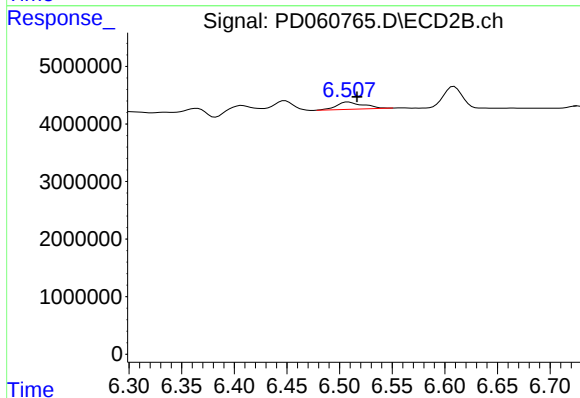


#13 Dieldrin

R.T.: 6.508 min
Delta R.T.: -0.008 min
Response: 2211117
Conc: 0.40 ng/ml

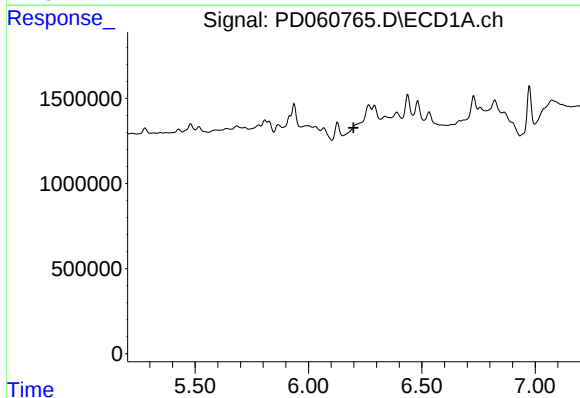


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.199 min
Response: 0
Conc: N.D.

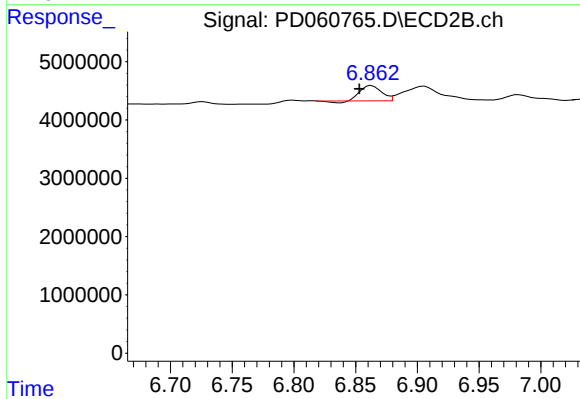

#16 4,4'-DDD


R.T.: 6.863 min
Delta R.T.: 0.010 min
Response: 3020170
Conc: 0.69 ng/ml

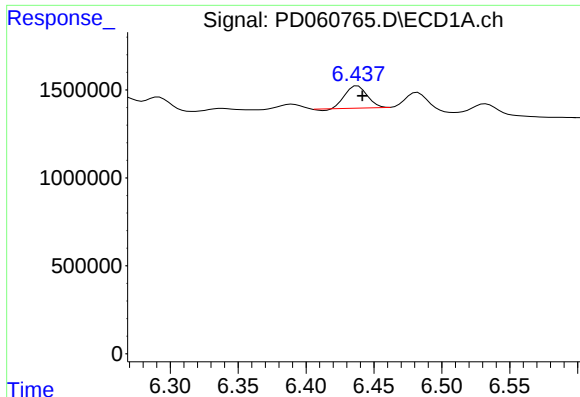

#17 4,4'-DDT


R.T.: 6.438 min
Delta R.T.: -0.003 min
Response: 1409903
Conc: 1.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

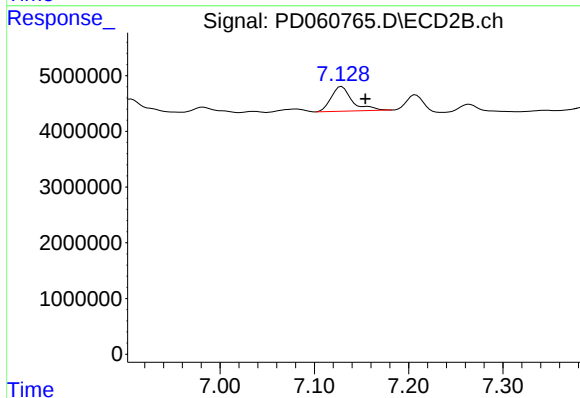


#17 4,4'-DDT

R.T.: 7.129 min
Delta R.T.: -0.025 min
Response: 6860775
Conc: 1.54 ng/ml

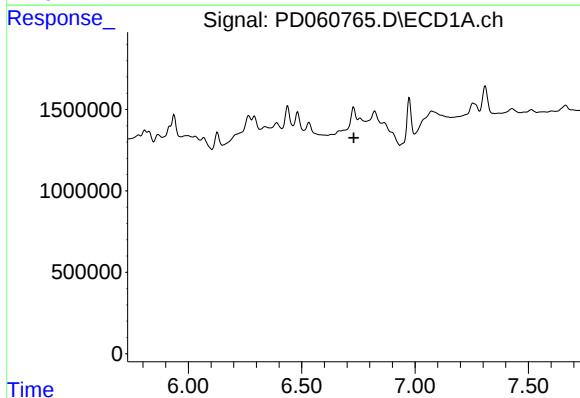


#19 Endosulfan Sulfate

R.T.: 6.729 min
Delta R.T.: 0.000 min
Response: -171440
Conc: N.D.

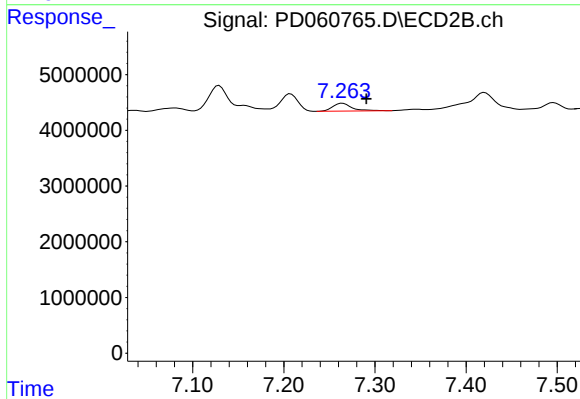

#19 Endosulfan Sulfate


R.T.: 7.265 min
Delta R.T.: -0.026 min
Response: 2038049
Conc: 0.46 ng/ml

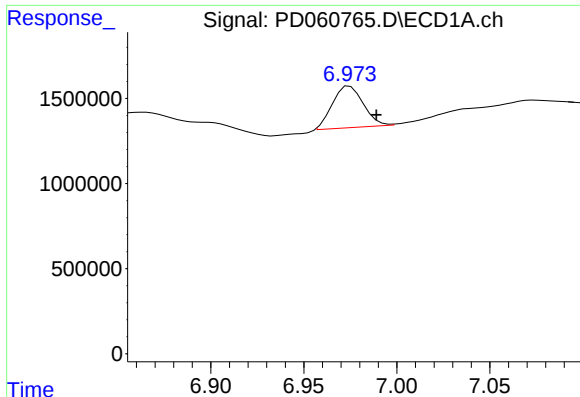

#20 Methoxychlor


R.T.: 6.975 min
Delta R.T.: -0.014 min
Response: 2806568
Conc: 3.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

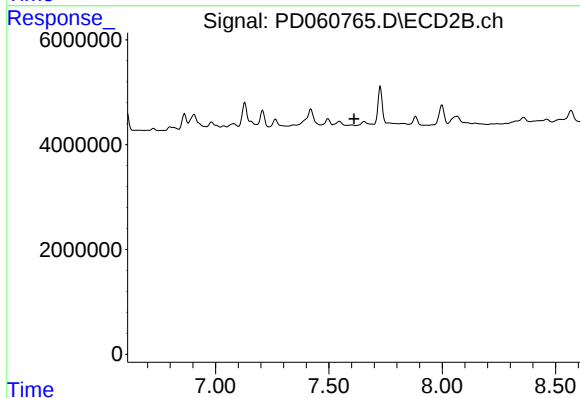


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.611 min
Response: 0
Conc: N.D.

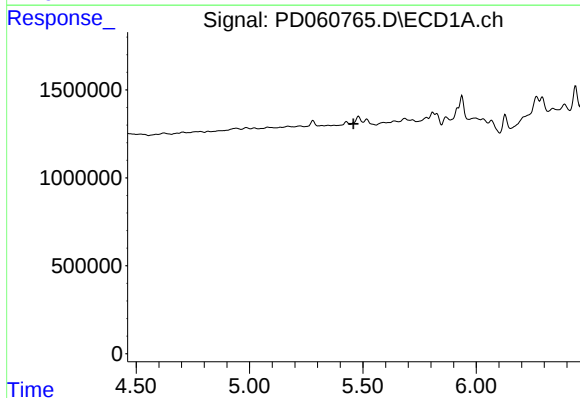


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.459 min
Response: 0
Conc: N.D.

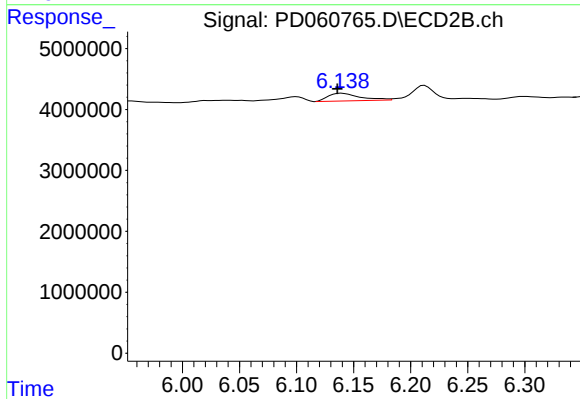

#25 Chlordane-3


R.T.: 6.139 min
Delta R.T.: 0.003 min
Response: 2456018
Conc: 3.46 ng/ml

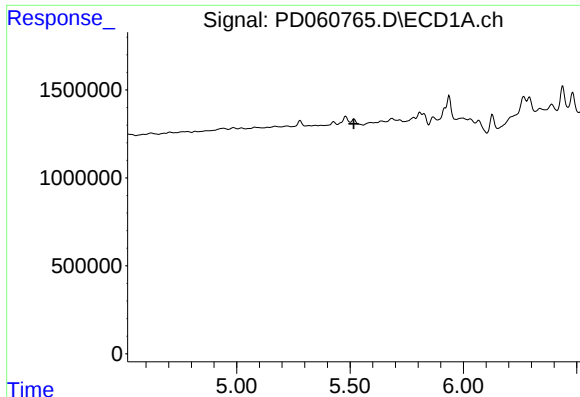

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.517 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

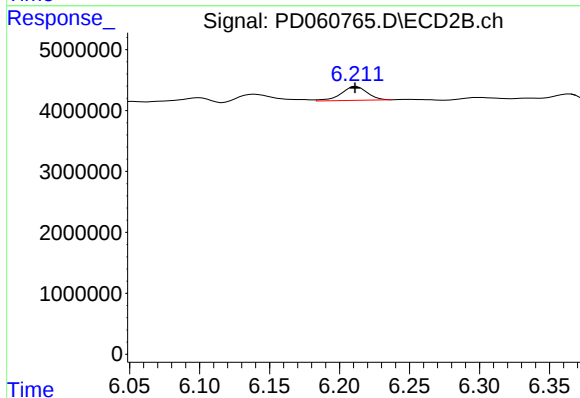


#26 Chlordane-4

R.T.: 6.212 min
Delta R.T.: 0.001 min
Response: 2937681
Conc: 3.55 ng/ml

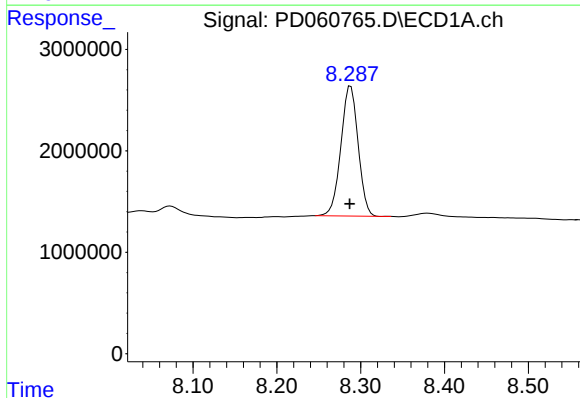

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: 0.001 min
Response: 18303552
Conc: 12.96 ng/ml

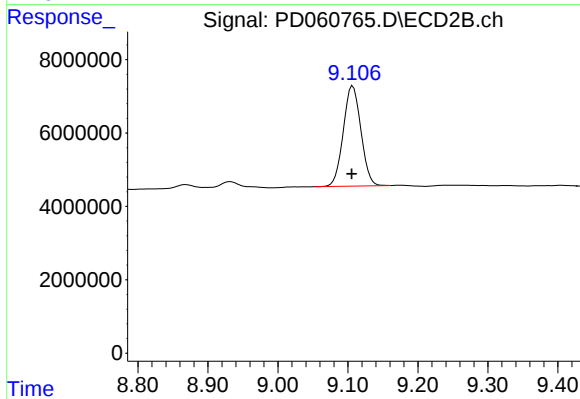

#28 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.002 min
Response: 47780350
Conc: 12.79 ng/ml