

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121720\
 Data File : PD060779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 16:11
 Operator : DD\AJ
 Sample : L5036-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 03:07:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 03:53:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.501	4.022	18764477	84001118	17.259	17.875
28)	SA Decachlor...	8.288	9.107	12081846	32620265	8.552	8.731
Target Compounds							
3)	MA gamma-BHC...	4.226	0.000	1975891	0	1.206	N.D. #
4)	MA Heptachlor	0.000	5.218	0	1318013	N.D.	0.202 #
5)	MB Aldrin	0.000	5.524	0	4373201	N.D.	0.717 #
6)	B beta-BHC	4.445f	4.863	2805328	1564805	3.966	0.563 #
7)	B delta-BHC	0.000	5.060f	0	8130713	N.D.	1.280 #
8)	B Heptachlo...	0.000	5.931f	0	3172280	N.D.	0.568 #
11)	B alpha-Chl...	5.504	0.000	1699491	0	1.100	N.D. #
25)	Chlordane-3	5.504f	0.000	1699491	0	12.512	N.D. #
26)	Chlordane-4	5.504	0.000	1699491	0	15.465	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121720\
Data File : PD060779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 16:11
Operator : DD\AJ
Sample : L5036-12
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 03:07:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 03:53:08 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

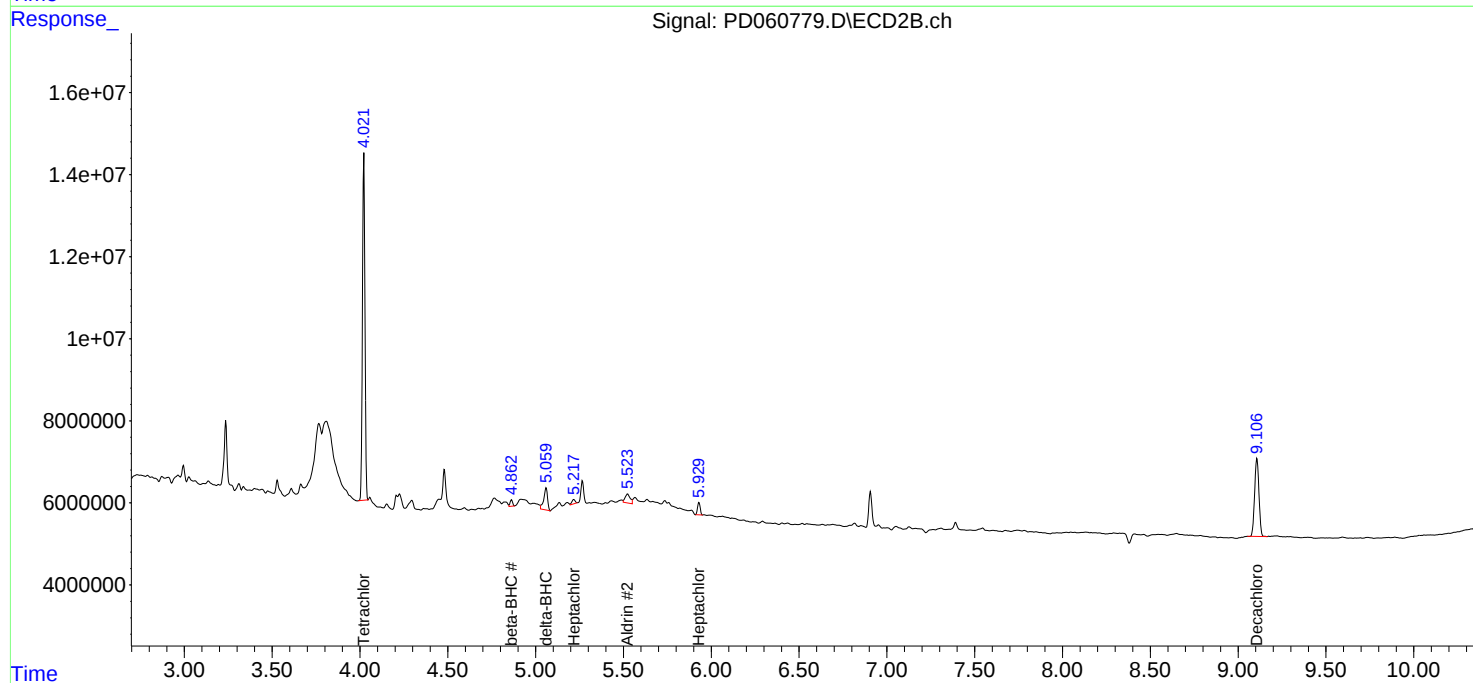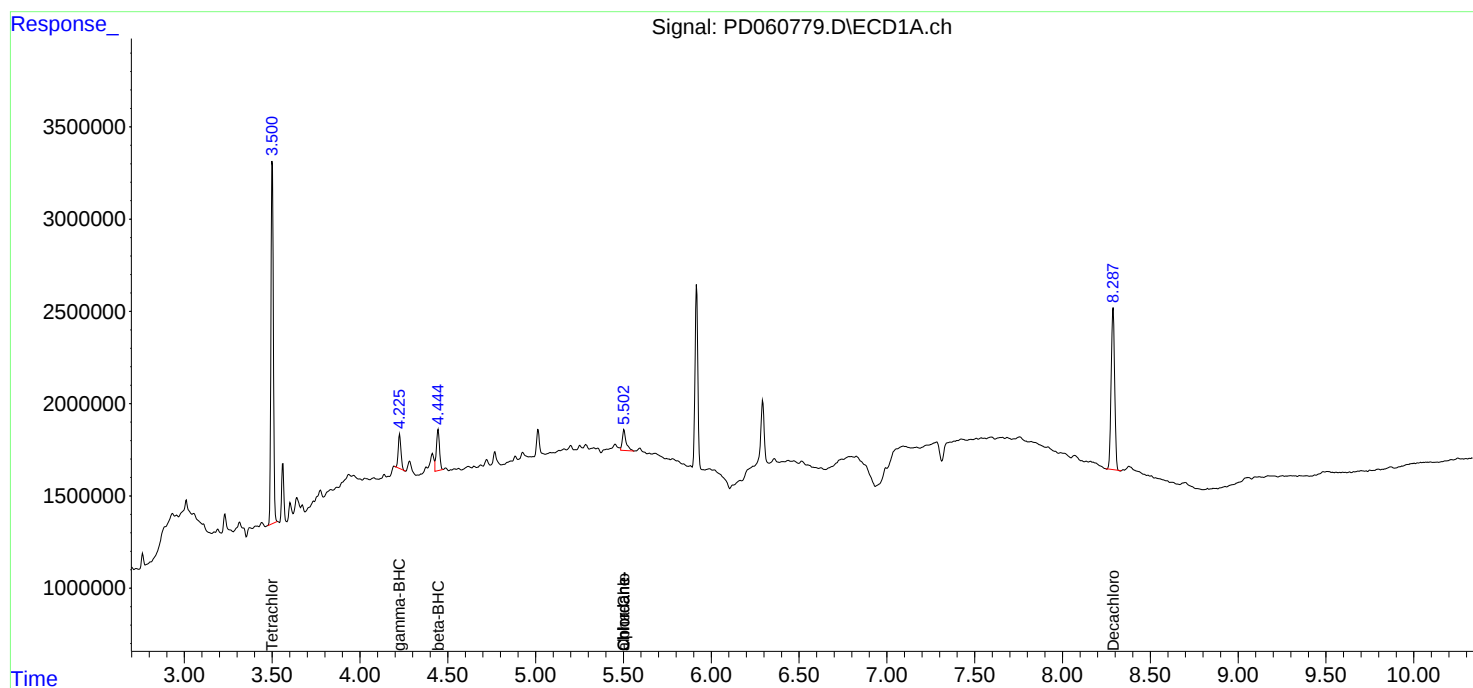


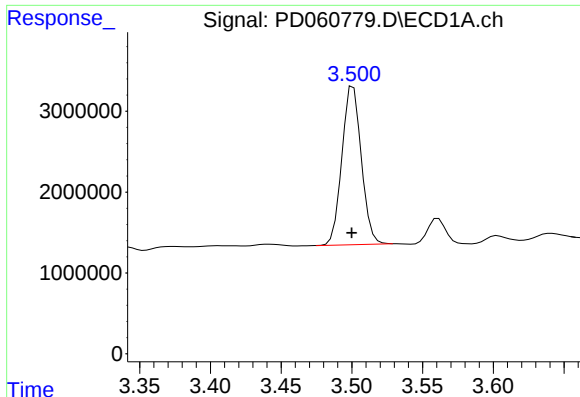

#1 Tetrachloro-m-xylene


R.T.: 3.501 min
Delta R.T.: 0.001 min
Response: 18764477
Conc: 17.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

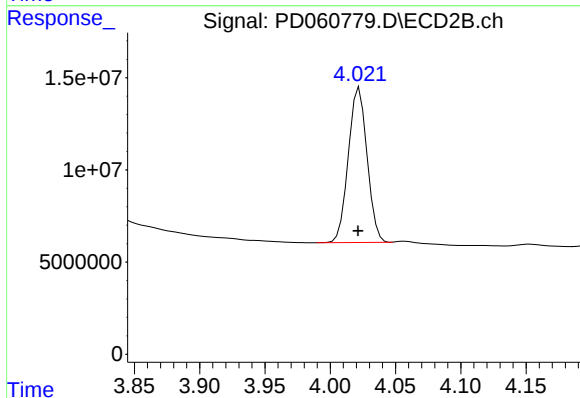


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.001 min
Response: 84001118
Conc: 17.87 ng/ml

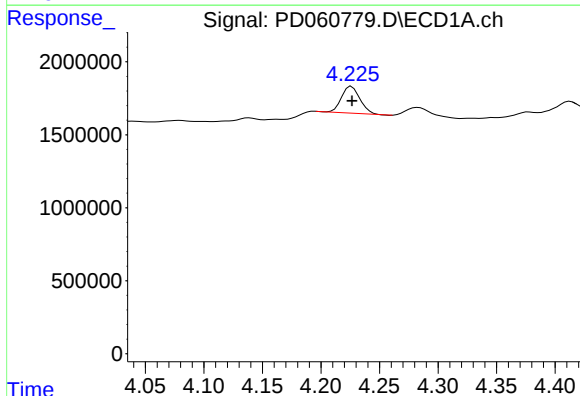


#3 gamma-BHC (Lindane)

R.T.: 4.226 min
Delta R.T.: 0.000 min
Response: 1975891
Conc: 1.21 ng/ml

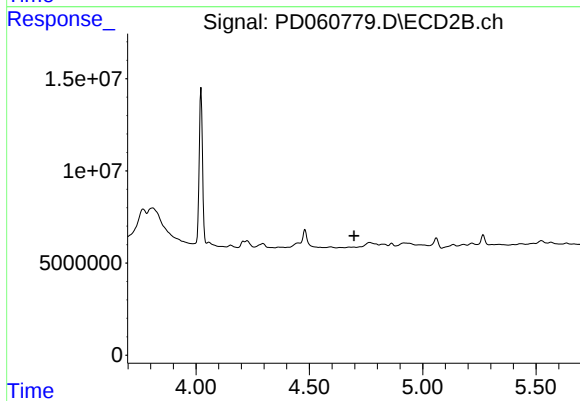

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.697 min
Response: 0
Conc: N.D.

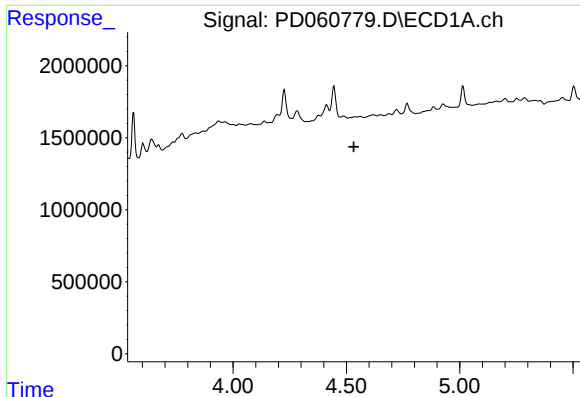

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.533 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

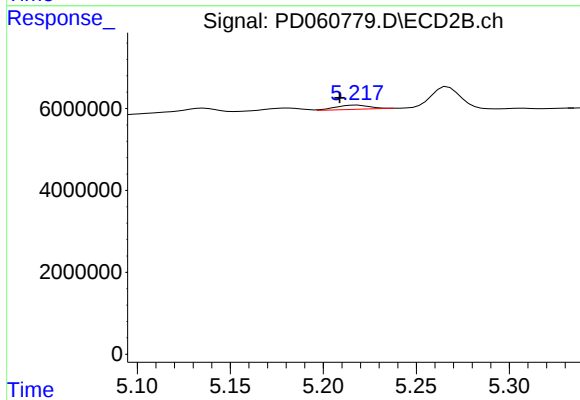


#4 Heptachlor

R.T.: 5.218 min
Delta R.T.: 0.009 min
Response: 1318013
Conc: 0.20 ng/ml

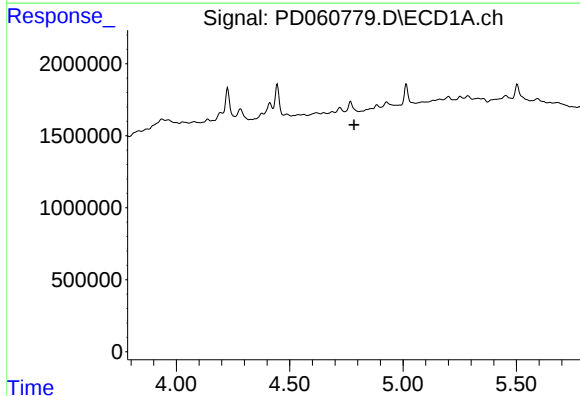


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 4.784 min
Response: 0
Conc: N.D.

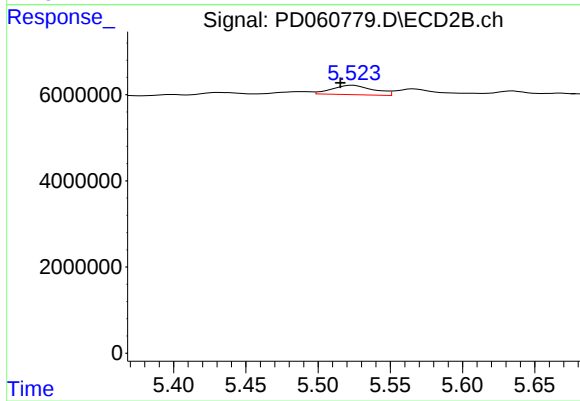

#5 Aldrin


R.T.: 5.524 min
Delta R.T.: 0.009 min
Response: 4373201
Conc: 0.72 ng/ml

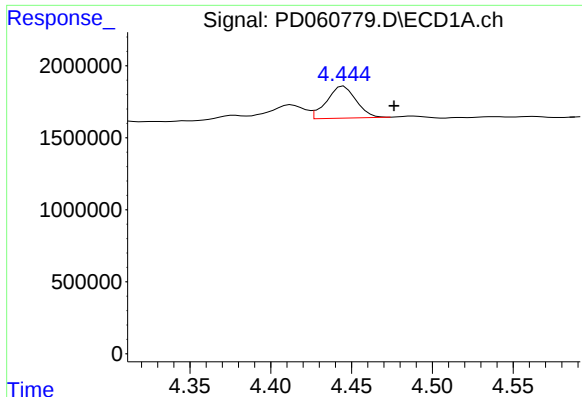

#6 beta-BHC


R.T.: 4.445 min
Delta R.T.: -0.031 min
Response: 2805328
Conc: 3.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

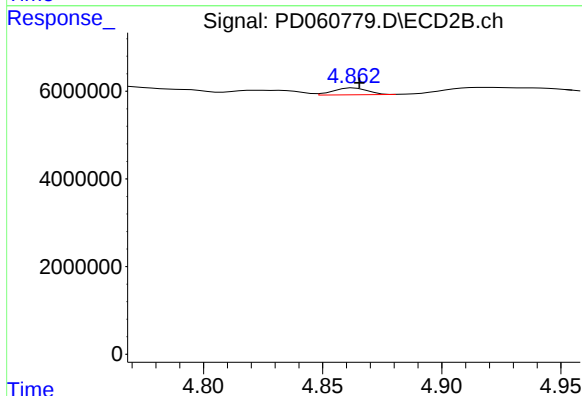


#6 beta-BHC

R.T.: 4.863 min
Delta R.T.: -0.002 min
Response: 1564805
Conc: 0.56 ng/ml

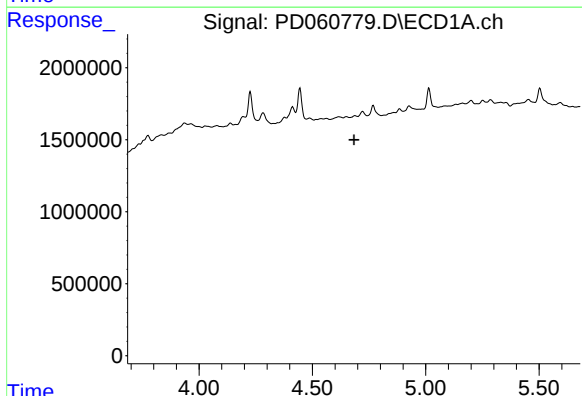


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.684 min
Response: 0
Conc: N.D.

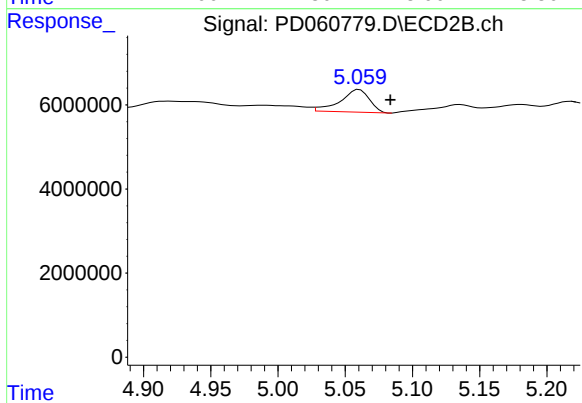

#7 delta-BHC


R.T.: 5.060 min
Delta R.T.: -0.023 min
Response: 8130713
Conc: 1.28 ng/ml

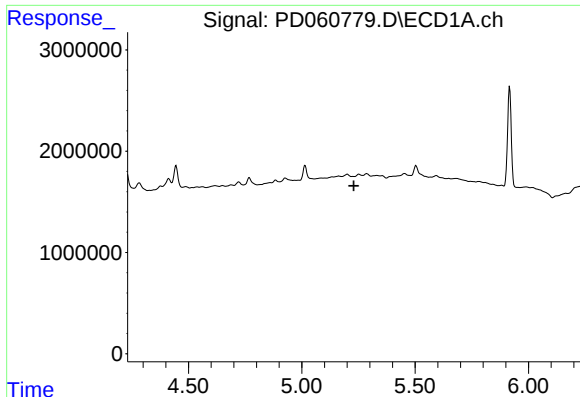

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

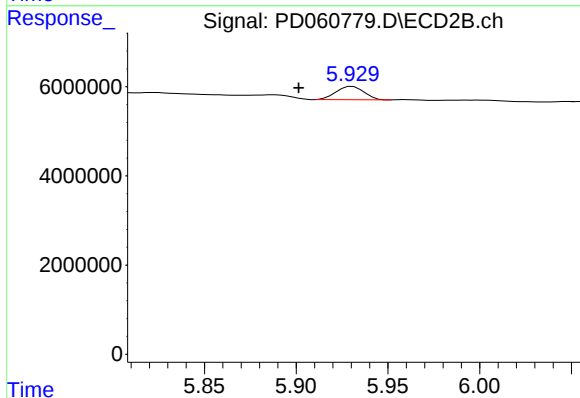


#8 Heptachlor epoxide

R.T.: 5.931 min
Delta R.T.: 0.029 min
Response: 3172280
Conc: 0.57 ng/ml

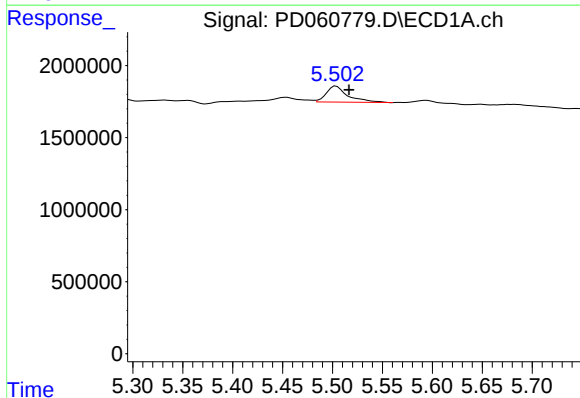


#11 alpha-Chlordane

R.T.: 5.504 min
Delta R.T.: -0.013 min
Response: 1699491
Conc: 1.10 ng/ml

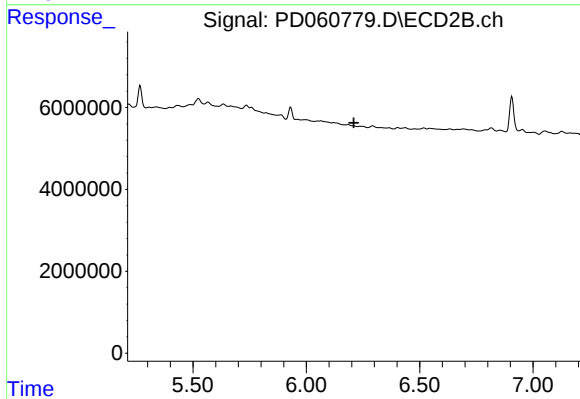

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.209 min
Response: 0
Conc: N.D.

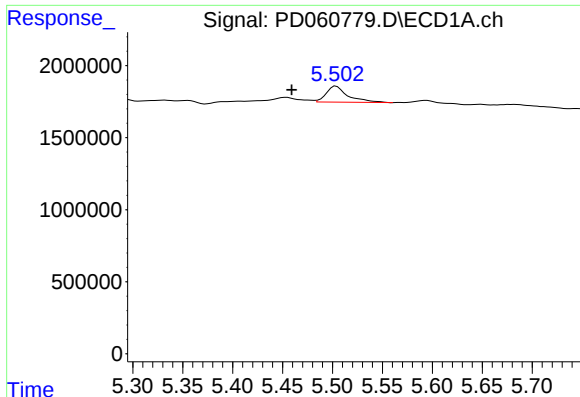

#25 Chlordane-3


R.T.: 5.504 min
Delta R.T.: 0.045 min
Response: 1699491
Conc: 12.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

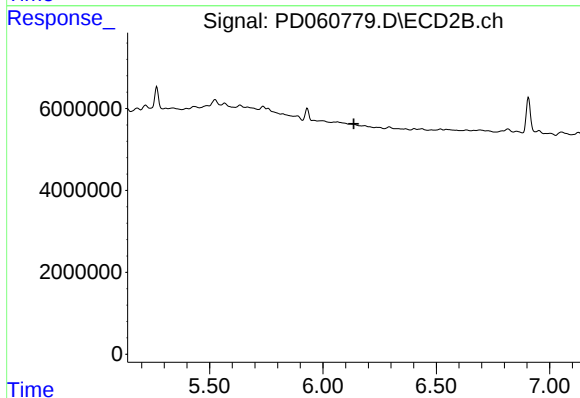


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.136 min
Response: 0
Conc: N.D.

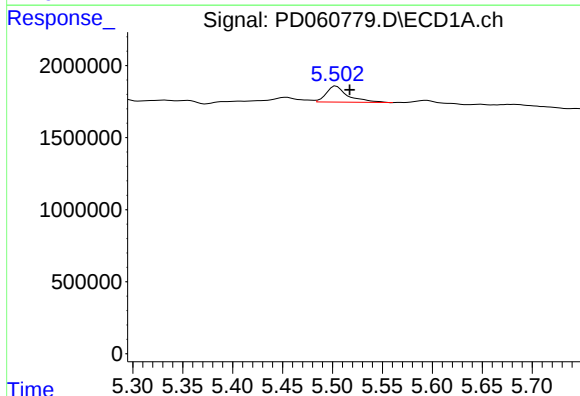


#26 Chlordane-4

R.T.: 5.504 min
Delta R.T.: -0.014 min
Response: 1699491
Conc: 15.47 ng/ml

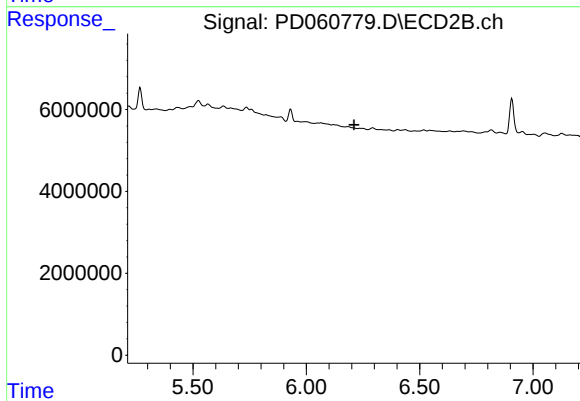

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.211 min
Response: 0
Conc: N.D.

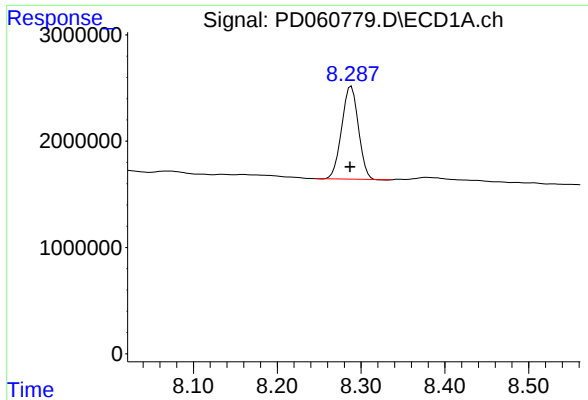

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: 0.001 min
Response: 12081846
Conc: 8.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

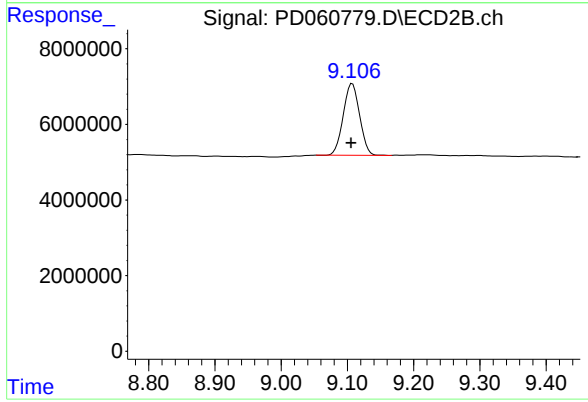

#28 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.002 min
Response: 32620265
Conc: 8.73 ng/ml