

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121720\
 Data File : PD060780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2020 16:26
 Operator : DD\AJ
 Sample : L5115-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 03:07:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 03:53:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	4.497f	4.873	1544630	28935547	2.184	10.419 #
7) B	delta-BHC	0.000	5.060f	0	14682920	N.D.	2.311 #
10) B	gamma-Chl...	5.471	0.000	1952767	0	1.263	N.D. #
12) B	4,4'-DDE	0.000	6.371	0	3142468	N.D.	0.594 #
13) MA	Dieldrin	0.000	6.529	0	2085111	N.D.	0.373 #
15) B	Endosulfa...	0.000	6.943	0	2785239	N.D.	0.560 #
18) B	Endrin al...	0.000	7.078	0	2588180	N.D.	0.637 #
23)	Chlordane-1	4.380	5.012	32010512	9486000	793.334	51.964 #
24)	Chlordane-2	0.000	5.467f	0	1127563	N.D.	5.862 #
25)	Chlordane-3	5.471	0.000	1952767	0	14.377	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121720\
Data File : PD060780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2020 16:26
Operator : DD\AJ
Sample : L5115-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 03:07:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 03:53:08 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

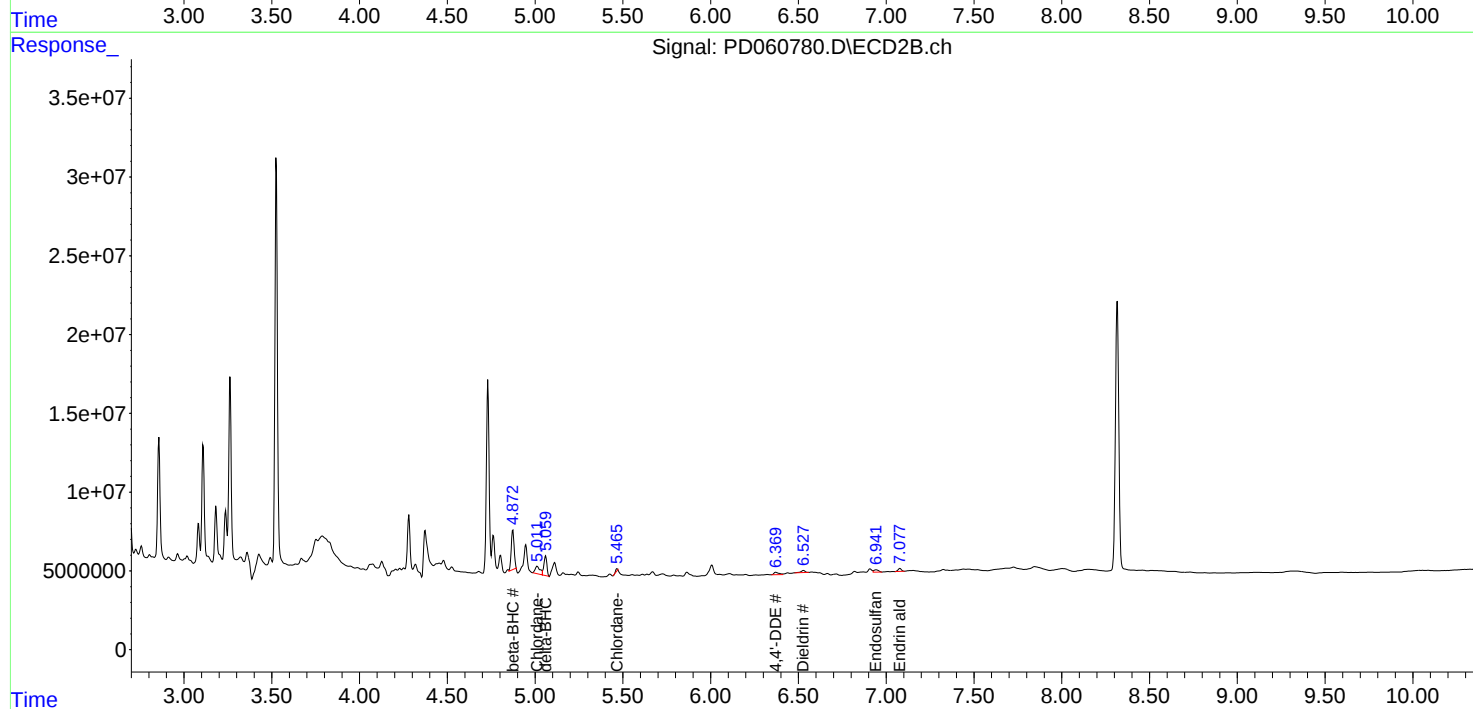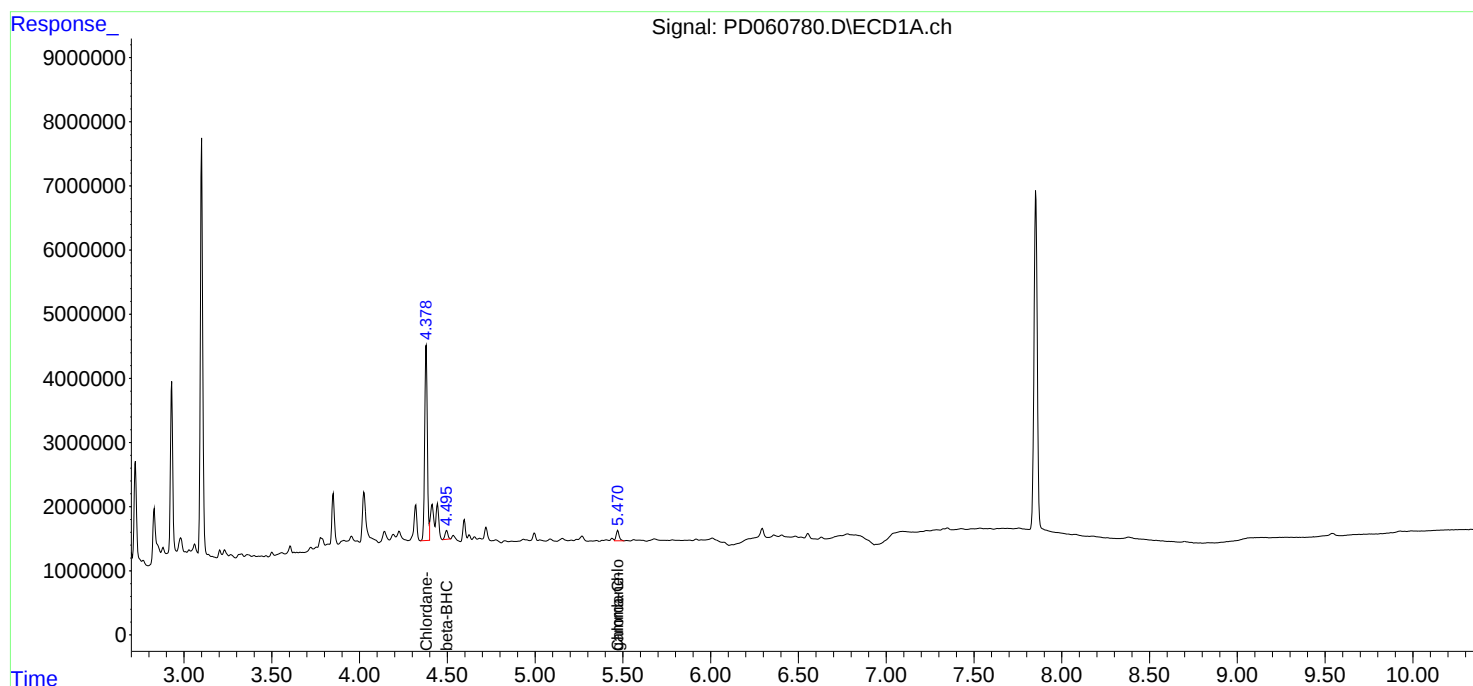


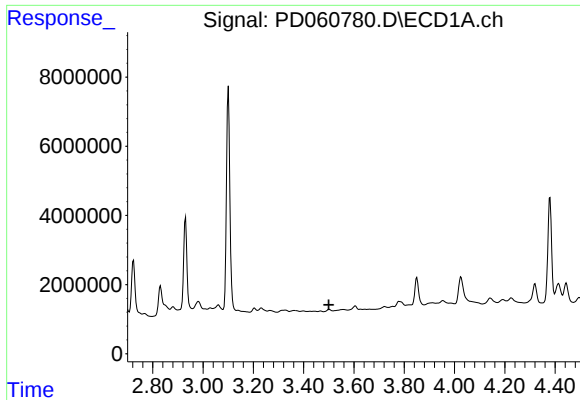

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

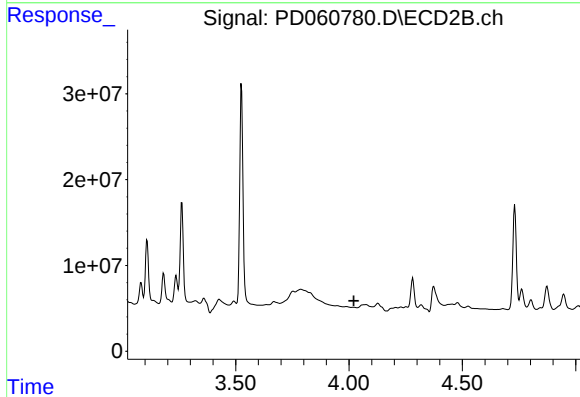


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.021 min
Response: 0
Conc: N.D.

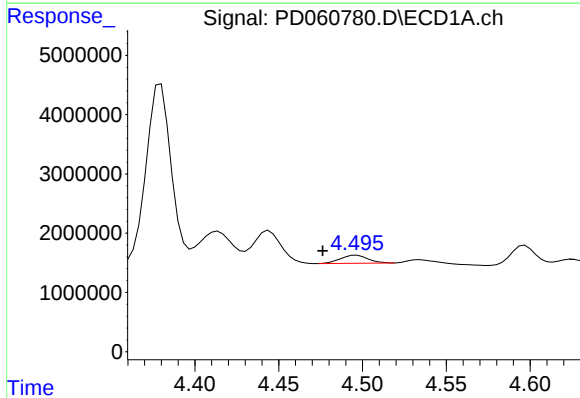


#6 beta-BHC

R.T.: 4.497 min
Delta R.T.: 0.020 min
Response: 1544630
Conc: 2.18 ng/ml

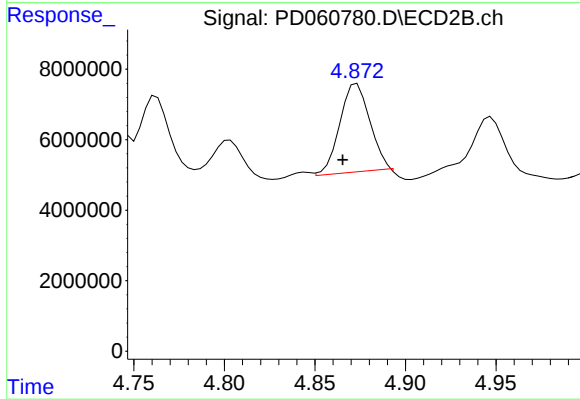

#6 beta-BHC


R.T.: 4.873 min
Delta R.T.: 0.008 min
Response: 28935547
Conc: 10.42 ng/ml

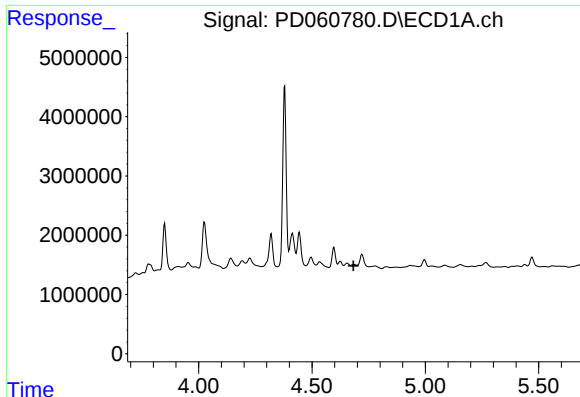

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.684 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

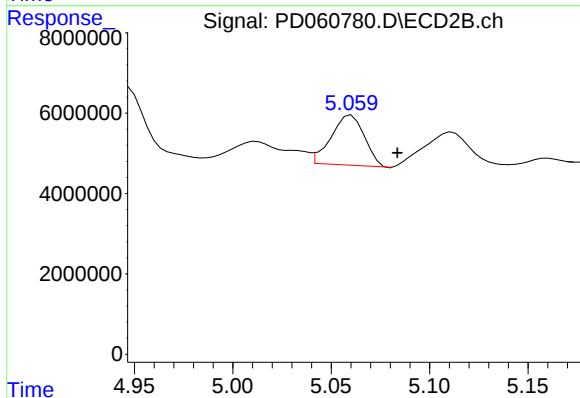


#7 delta-BHC

R.T.: 5.060 min
Delta R.T.: -0.023 min
Response: 14682920
Conc: 2.31 ng/ml

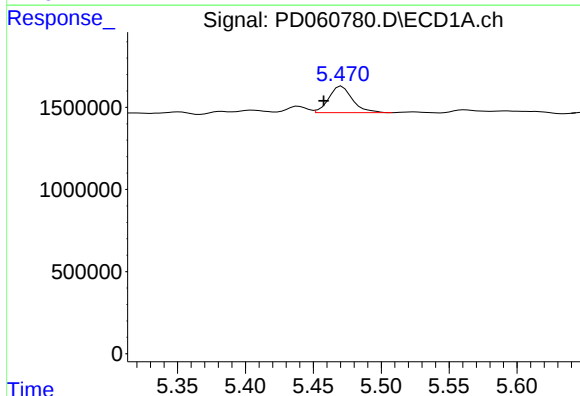


#10 gamma-Chlordane

R.T.: 5.471 min
Delta R.T.: 0.013 min
Response: 1952767
Conc: 1.26 ng/ml

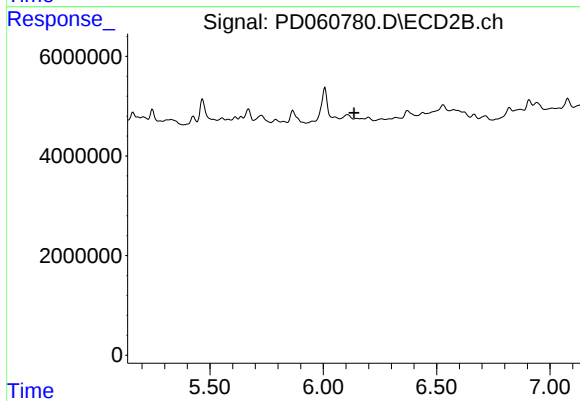

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.136 min
Response: 0
Conc: N.D.

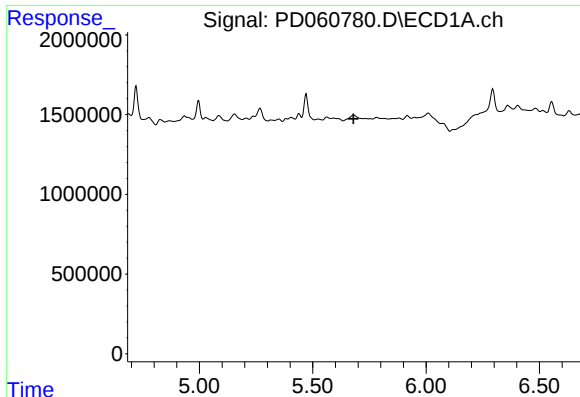

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

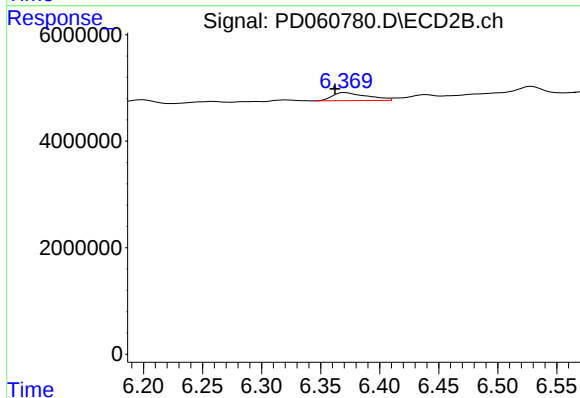


#12 4,4'-DDE

R.T.: 6.371 min
Delta R.T.: 0.009 min
Response: 3142468
Conc: 0.59 ng/ml

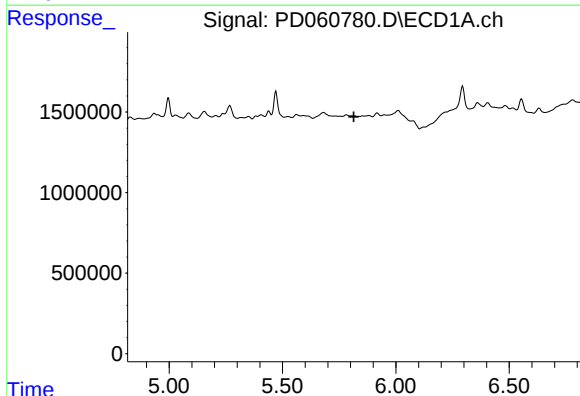


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.815 min
Response: 0
Conc: N.D.

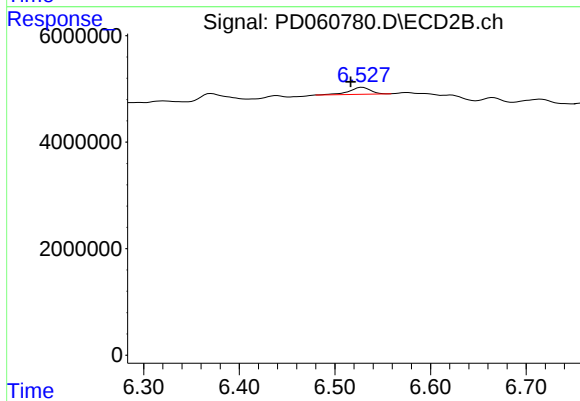

#13 Dieldrin


R.T.: 6.529 min
Delta R.T.: 0.012 min
Response: 2085111
Conc: 0.37 ng/ml

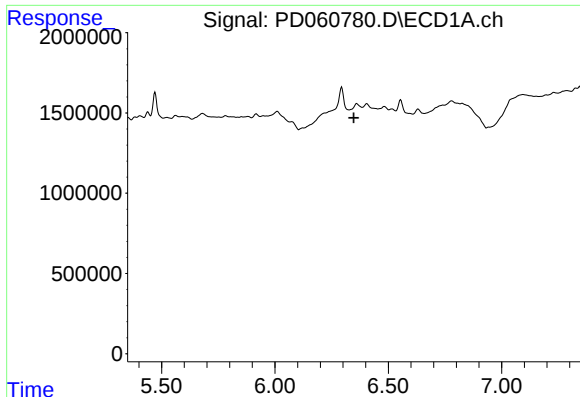

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.348 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

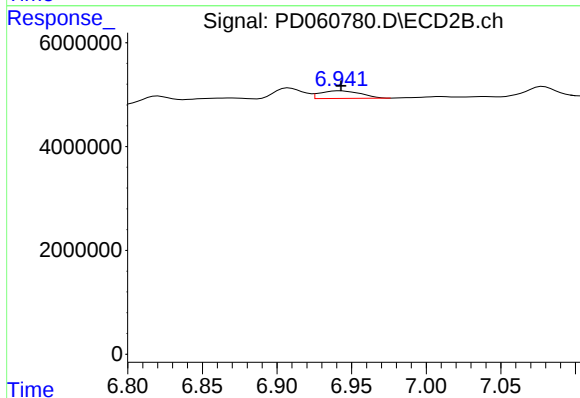


#15 Endosulfan II

R.T.: 6.943 min
Delta R.T.: 0.000 min
Response: 2785239
Conc: 0.56 ng/ml

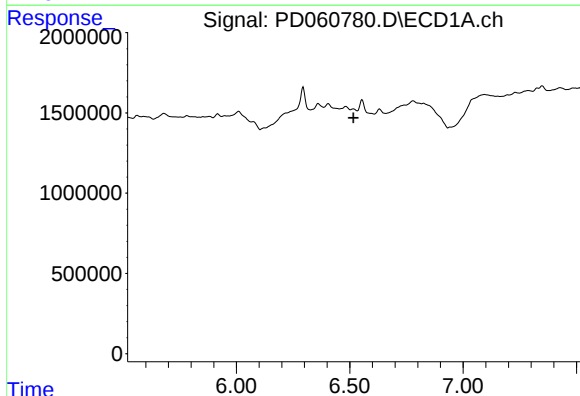


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.517 min
Response: 0
Conc: N.D.

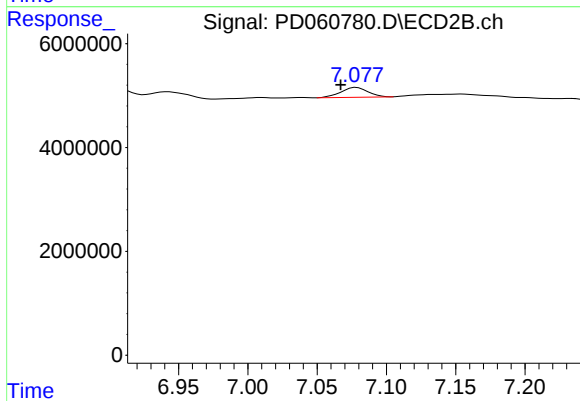

#18 Endrin aldehyde


R.T.: 7.078 min
Delta R.T.: 0.011 min
Response: 2588180
Conc: 0.64 ng/ml

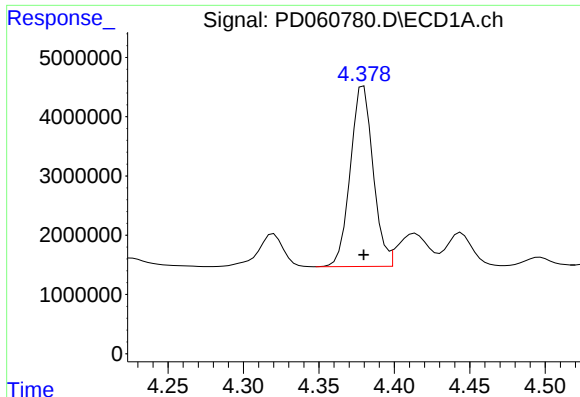

#23 Chlordane-1


R.T.: 4.380 min
Delta R.T.: 0.000 min
Response: 32010512
Conc: 793.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

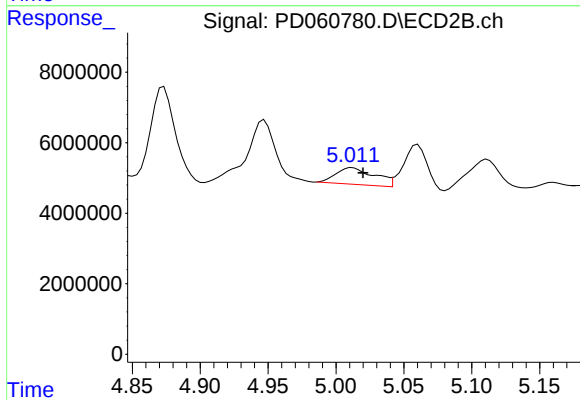


#23 Chlordane-1

R.T.: 5.012 min
Delta R.T.: -0.008 min
Response: 9486000
Conc: 51.96 ng/ml

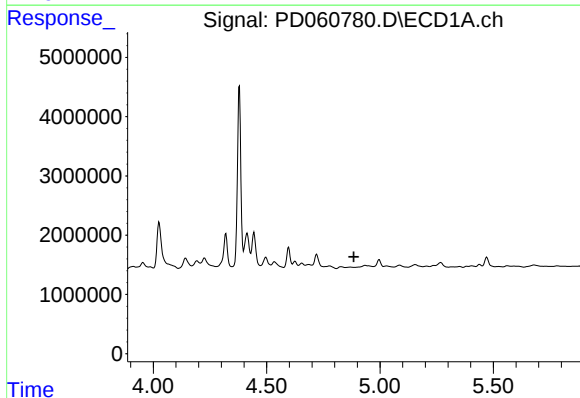


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

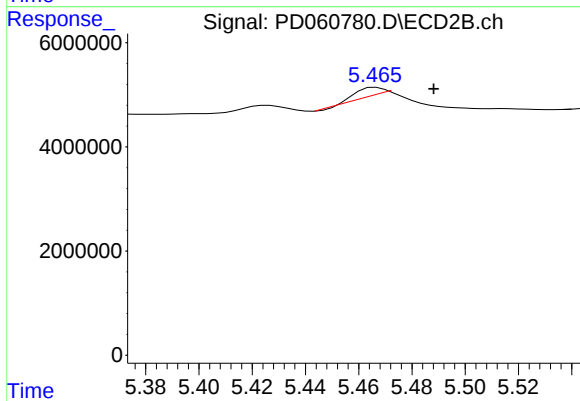

#24 Chlordane-2


R.T.: 5.467 min
Delta R.T.: -0.022 min
Response: 1127563
Conc: 5.86 ng/ml

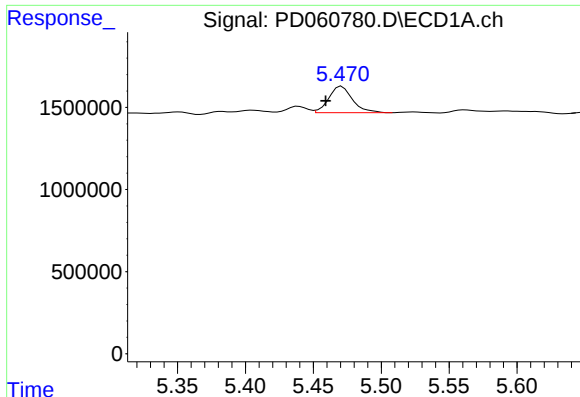

#25 Chlordane-3


R.T.: 5.471 min
Delta R.T.: 0.012 min
Response: 1952767
Conc: 14.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

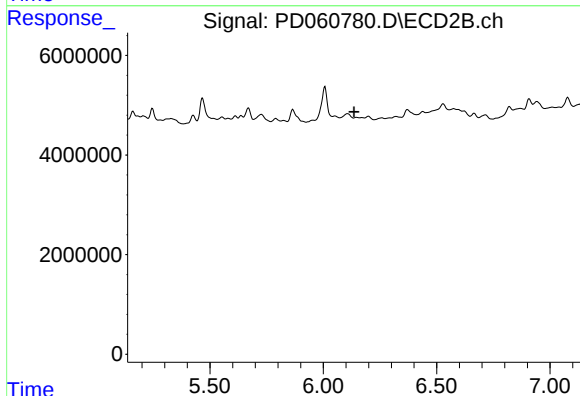


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.136 min
Response: 0
Conc: N.D.

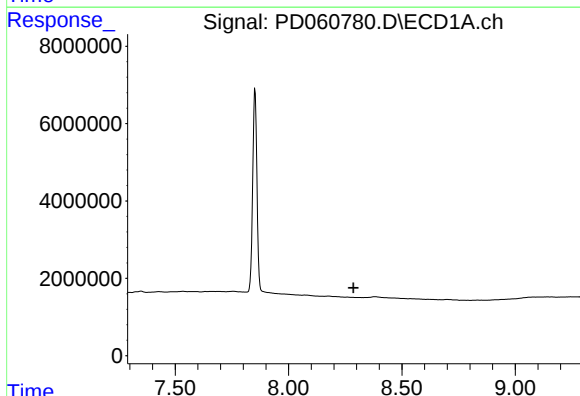

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.287 min
Response: 0
Conc: N.D.

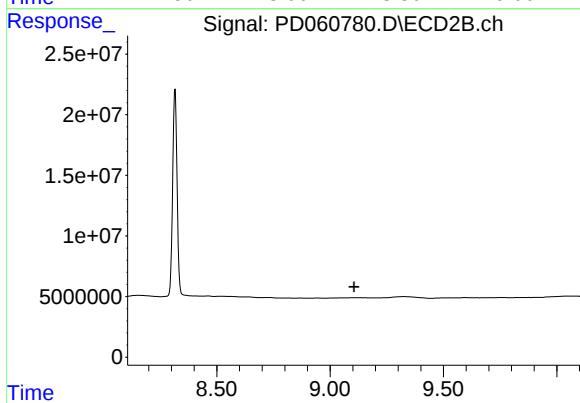

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.105 min
Response: 0
Conc: N.D.