

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121721\
 Data File : PD067419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2021 14:47
 Operator : AR\AJ
 Sample : M5034-06MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00V2MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/20/2021
 Supervised By : mohammad ahmed 12/20/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 07:53:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:28:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.966	32015050	217.3E6	14.662	27.121 #
2)	SA Decachlor...	8.157	9.025	25780988	153.2E6	22.708	30.213 #
Target Compounds							
2)	A alpha-BHC	3.871	4.358	133.9E6	533.9E6	40.952	49.765
3)	MA gamma-BHC...	4.152	4.643	136.1E6	530.2E6	42.779	52.855
4)	MA Heptachlor	4.445	5.143	156.0E6	491.6E6	48.670	52.707
5)	MB Aldrin	4.690	5.446	152.6E6	449.1E6	49.326	52.079
6)	B beta-BHC	4.401	4.820	64706342	241.5E6	48.606	52.335m
7)	B delta-BHC	4.603	5.036	25040006	105.0E6	8.754	11.858 #
8)	B Heptachlo...	5.131	5.836	137.7E6	346.7E6	49.867	49.468
9)	A Endosulfan I	5.466	6.193	122.3E6	372.9E6	46.001	51.437
10)	B trans-Chl...	5.354	6.070	140.9E6	395.3E6	49.994	52.081
11)	B cis-Chlor...	5.412	6.141	133.2E6	388.4E6	48.006	52.503
12)	B 4,4'-DDE	5.577	6.302	274.3E6	758.8E6	109.603	113.232
13)	MA Dieldrin	5.709	6.451	284.6E6	770.9E6	98.830	103.604
14)	MA Endrin	5.966	6.671	236.4E6	636.1E6	103.355	109.634
15)	B Endosulfa...	6.239	6.885	214.8E6	643.5E6	95.653	105.993
16)	A 4,4'-DDD	6.091	6.797	201.8E6	602.5E6	95.455	103.026
17)	MA 4,4'-DDT	6.330	7.094	201.1E6	580.4E6	94.624	100.728
18)	B Endrin al...	6.407	7.010	168.0E6	517.4E6	101.845	109.775
19)	B Endosulfa...	6.620	7.233	135.6E6	444.9E6	70.314	77.467
20)	A Methoxychlor	6.877	7.557	451.5E6	1375.8E6	454.294	494.322
21)	B Endrin ke...	7.111	7.707	196.9E6	689.3E6	94.851	104.385

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121721\
Data File : PD067419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2021 14:47
Operator : AR\AJ
Sample : M5034-06MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 07:53:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

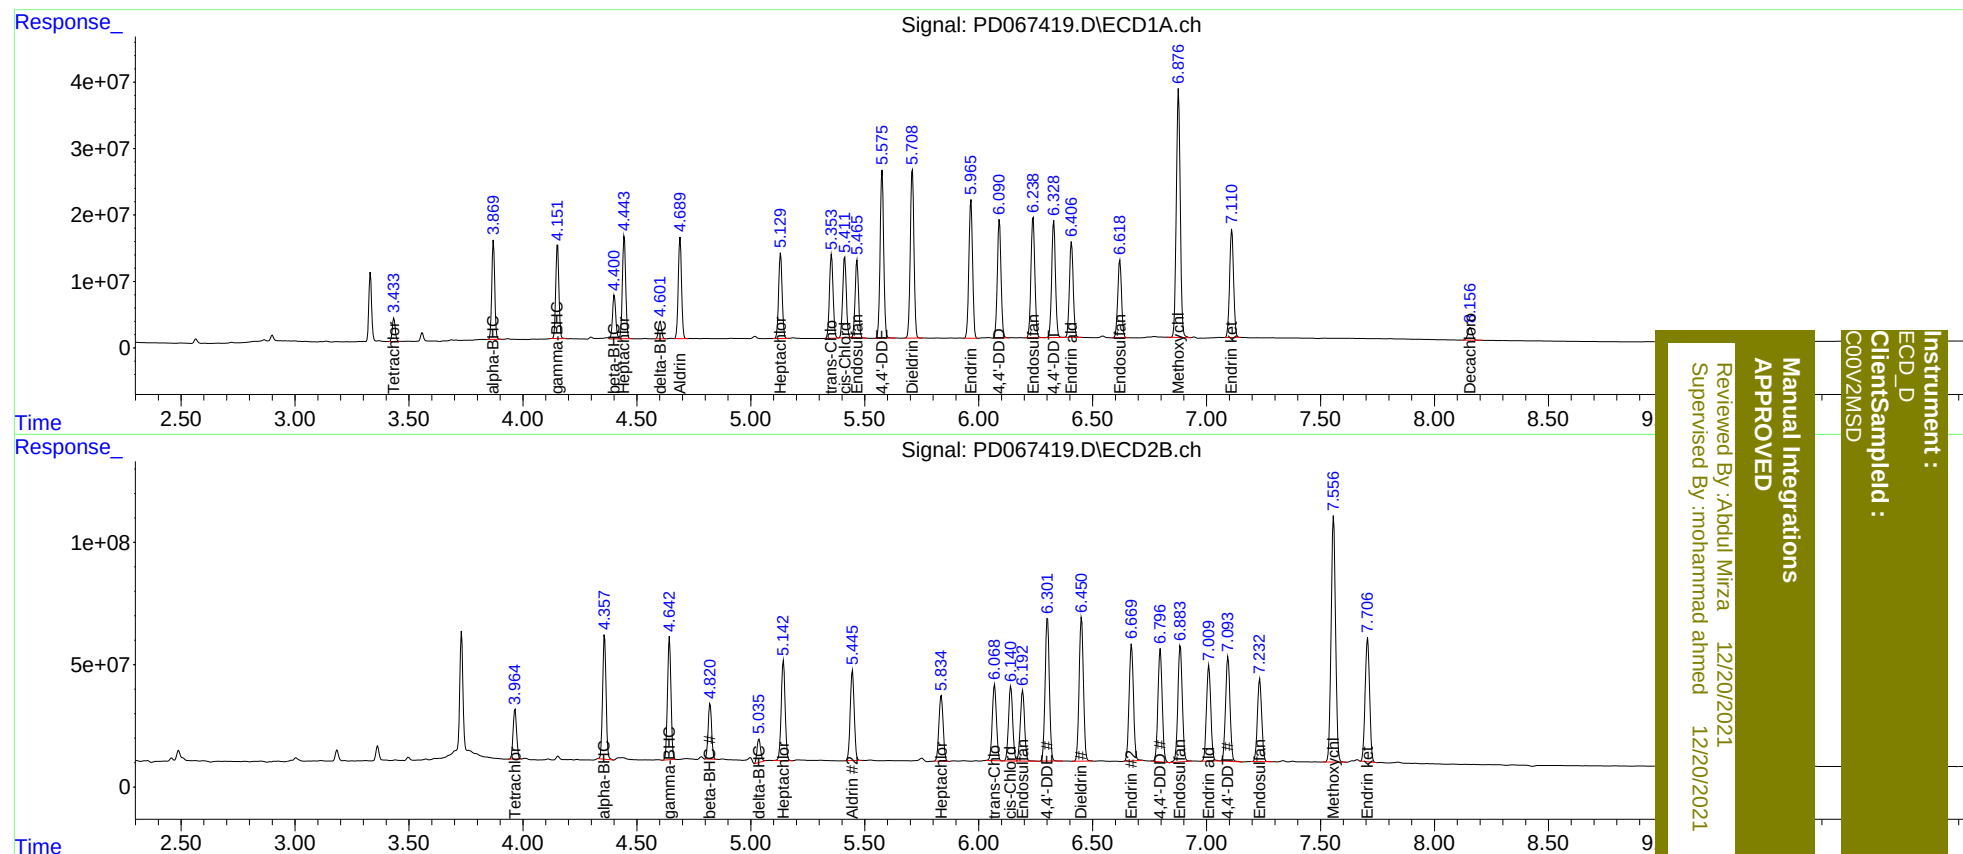

Instrument :
ECD_D
ClientSampled :
C00V2MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 12/20/2021
Supervised By: mohammad ahmed 12/20/2021