

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121721\
Data File : PD067416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2021 14:05
Operator : AR\AJ
Sample : M5034-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :

Manual IntegrationsAPPROVED

Reviewed By :
Supervised By :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 04:12:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

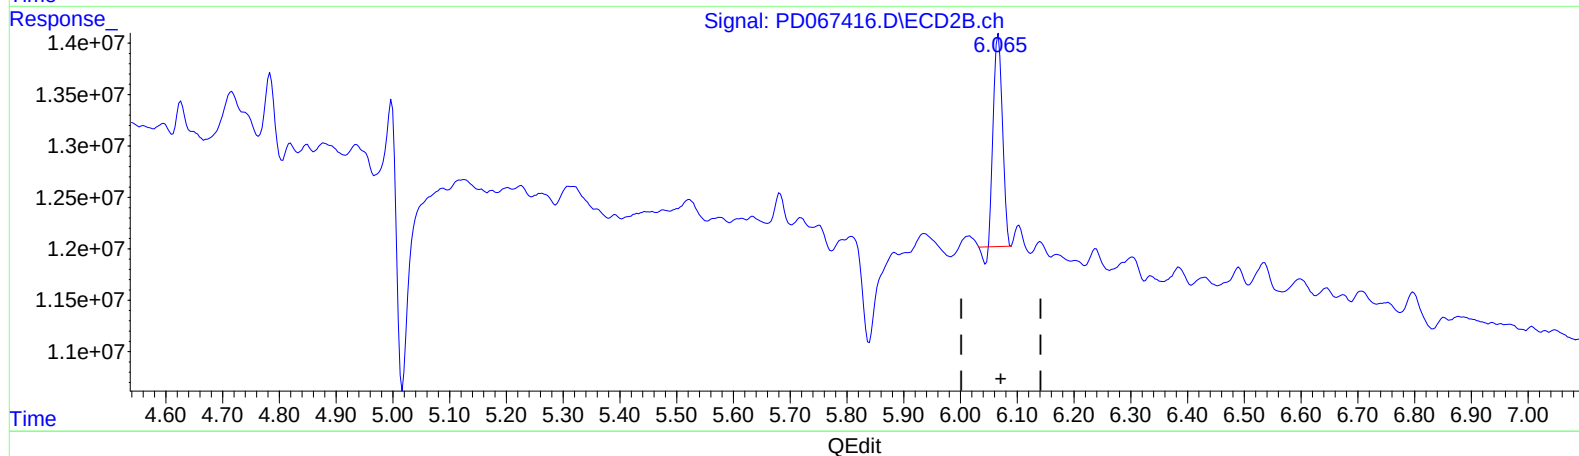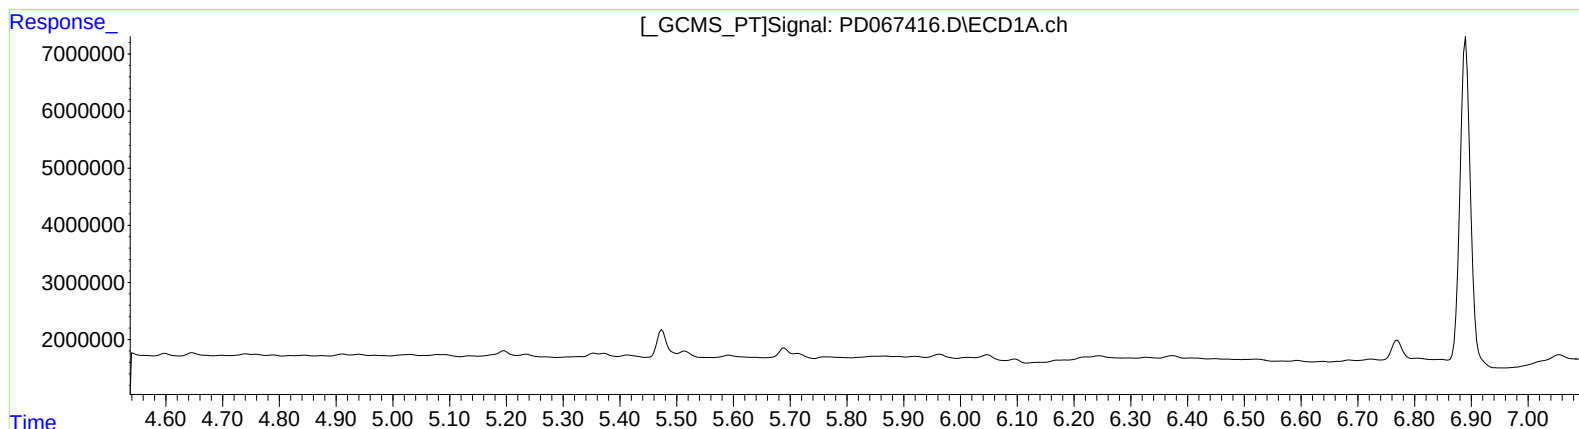

(10) trans-Chlordane (B)

0.000min 0.000 ng/ml

response 0

(10) trans-Chlordane #2 (B)

6.067min 2.968 ng/ml

response 22524911

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121721\
Data File : PD067416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2021 14:05
Operator : AR\AJ
Sample : M5034-03
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :

Manual IntegrationsAPPROVED

Reviewed By :
Supervised By :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 04:12:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

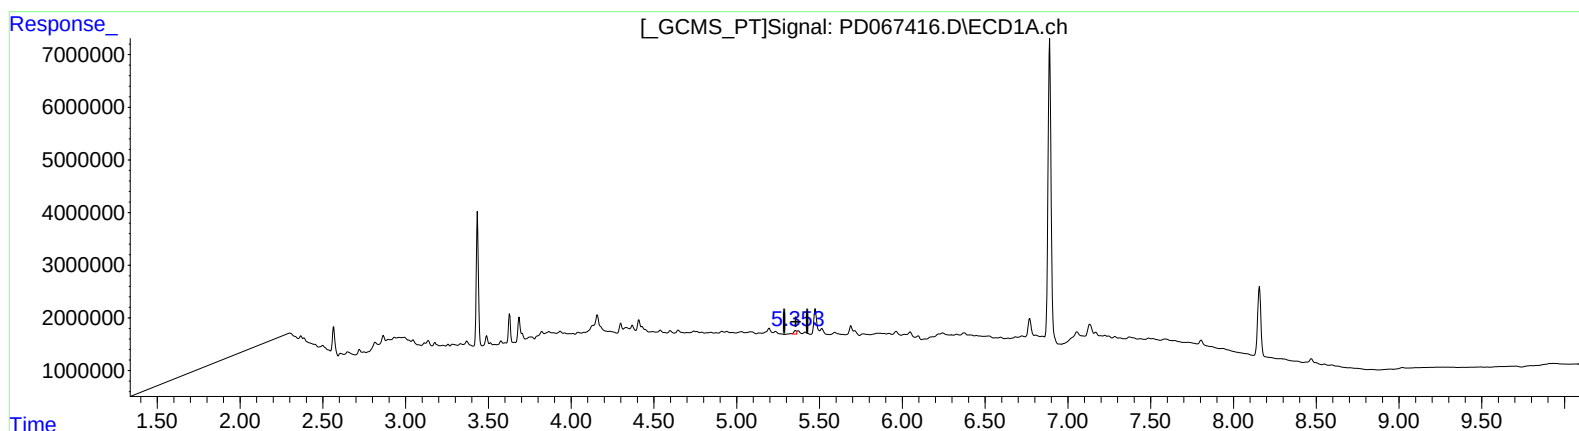

(10) trans-Chlordane (B)

5.353min 0.225 ng/ml m

response 634702

(10) trans-Chlordane #2 (B)

6.065min 3.556 ng/ml m

response 26989896