

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121721\
Data File : PD067417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2021 14:19
Operator : AR\AJ
Sample : M5034-04
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :

Manual IntegrationsAPPROVED

Reviewed By :
Supervised By :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 03:30:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

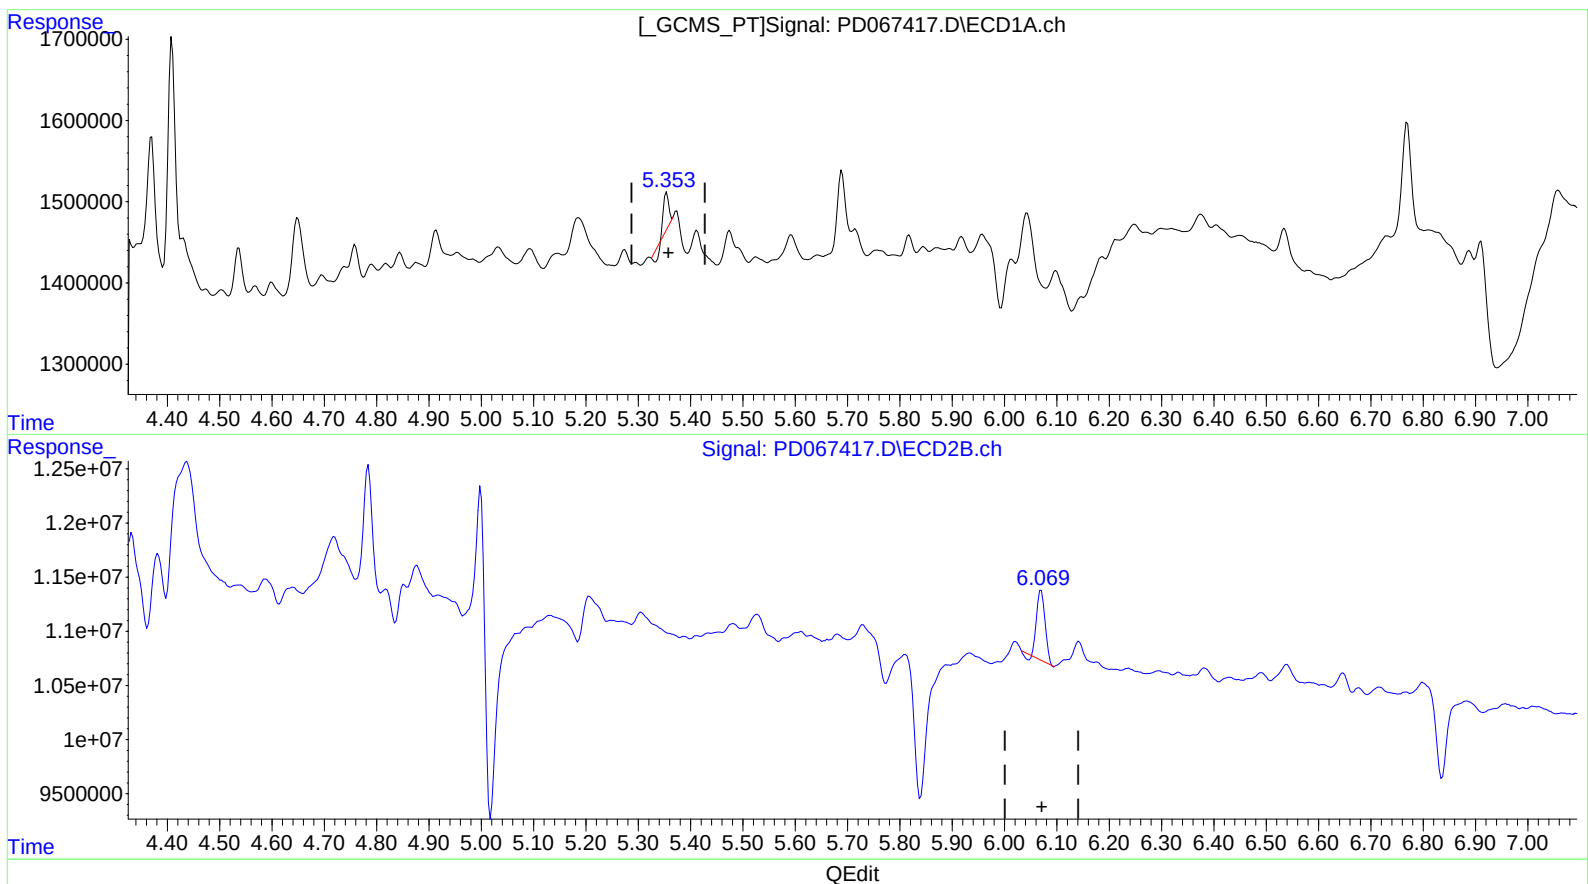

(10) trans-Chlordane (B)

5.355min 0.071 ng/ml

response 198948

(10) trans-Chlordane #2 (B)

6.070min 0.941 ng/ml

response 7143202

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121721\
Data File : PD067417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2021 14:19
Operator : AR\AJ
Sample : M5034-04
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :

Manual IntegrationsAPPROVED

Reviewed By :
Supervised By :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 03:30:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

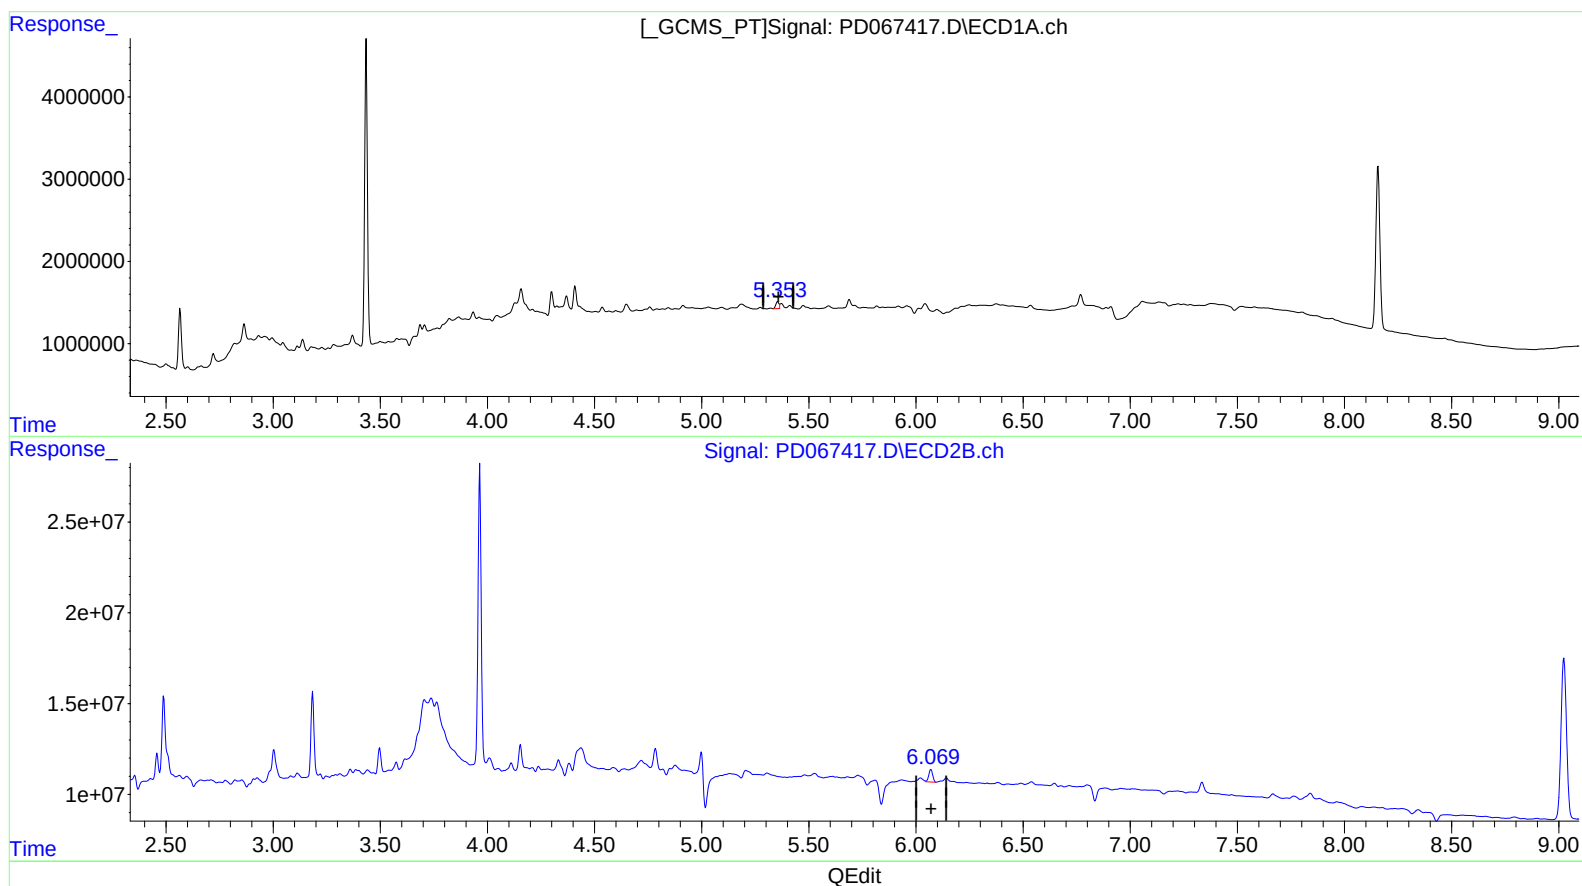

(10) trans-Chlordane (B)

5.353min 0.351 ng/ml m

response 989518

(10) trans-Chlordane #2 (B)

6.069min 1.148 ng/ml m

response 8710003

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121721\
Data File : PD067417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2021 14:19
Operator : AR\AJ
Sample : M5034-04
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :

Manual IntegrationsAPPROVED

Reviewed By :
Supervised By :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 03:30:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

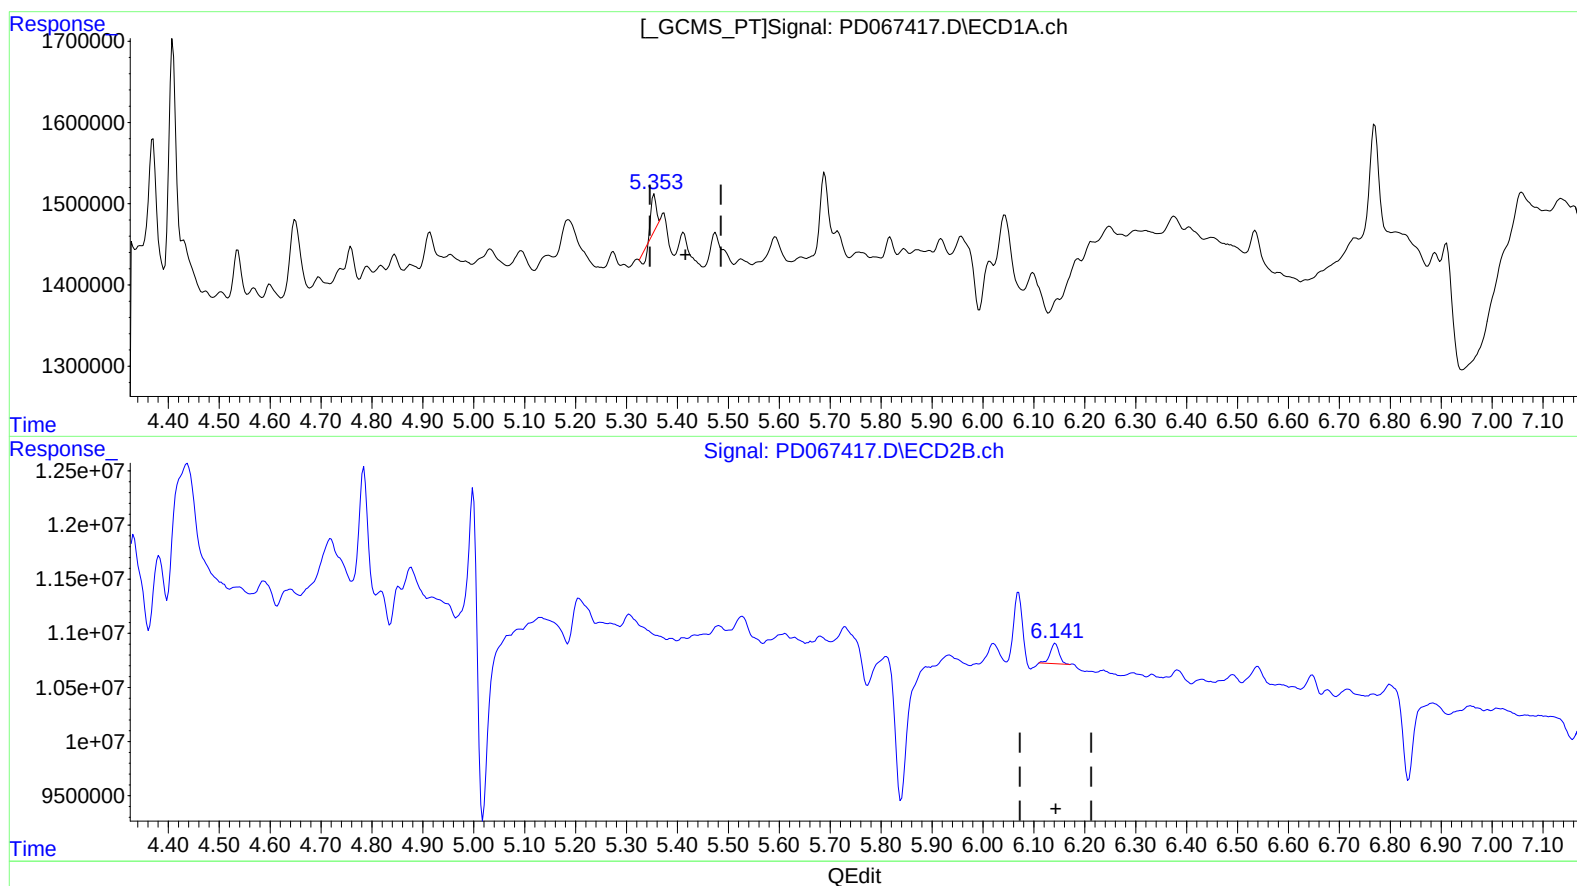

(11) cis-Chlordane (B)

5.355min 0.072 ng/ml

response 198948

(11) cis-Chlordane #2 (B)

6.142min 0.309 ng/ml

response 2283262

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121721\
Data File : PD067417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2021 14:19
Operator : AR\AJ
Sample : M5034-04
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :

Manual IntegrationsAPPROVED

Reviewed By :
Supervised By :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 03:30:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

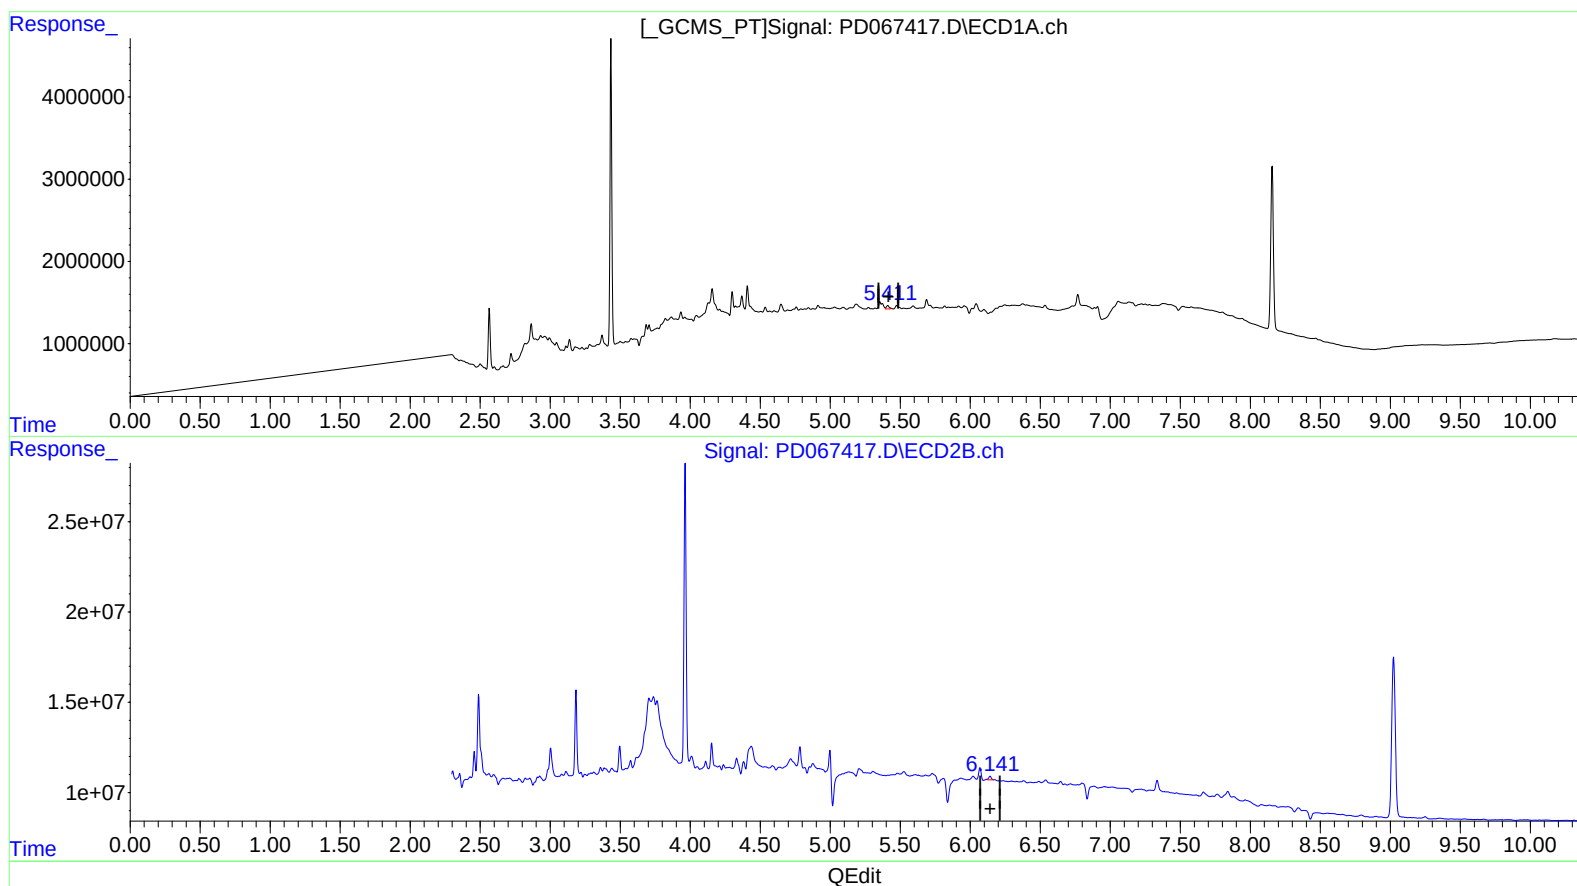

(11) cis-Chlordane (B)
5.411min 0.198 ng/ml m
response 549694

(11) cis-Chlordane #2 (B)
6.141min 0.335 ng/ml m
response 2480089