

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121723\
 Data File : PD080122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2023 22:49
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA1040

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 01:41:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 01:29:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.799	7522229	13099864	5.276	5.309
27)	SA Decachlor...	9.111	7.941	19717237	29481682	11.066	10.876
Target Compounds							
2)	A alpha-BHC	4.023	3.302	11444615	18600901	4.717	4.739
3)	MA gamma-BHC...	4.356	3.631	11155063	17791801	4.828	4.840
4)	MA Heptachlor	4.949	3.973	12234688	18121428	5.107	5.008
9)	A Endosulfan I	6.105	5.125	11020889	16219038	5.391	5.159
13)	MA Dieldrin	6.381	5.390	21295356	33698700	9.903	9.710
14)	MA Endrin	6.611	5.665	17882279	29703833	9.981	9.906
16)	A 4,4'-DDD	6.742	5.812	15672293	25635267	9.778	9.703
17)	MA 4,4'-DDT	7.057	6.063	16788538	26432383	9.756	9.510
20)	A Methoxychlor	7.531	6.638	47666681	76543925	53.252	55.242

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121723\
Data File : PD080122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 22:49
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 01:41:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 01:29:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

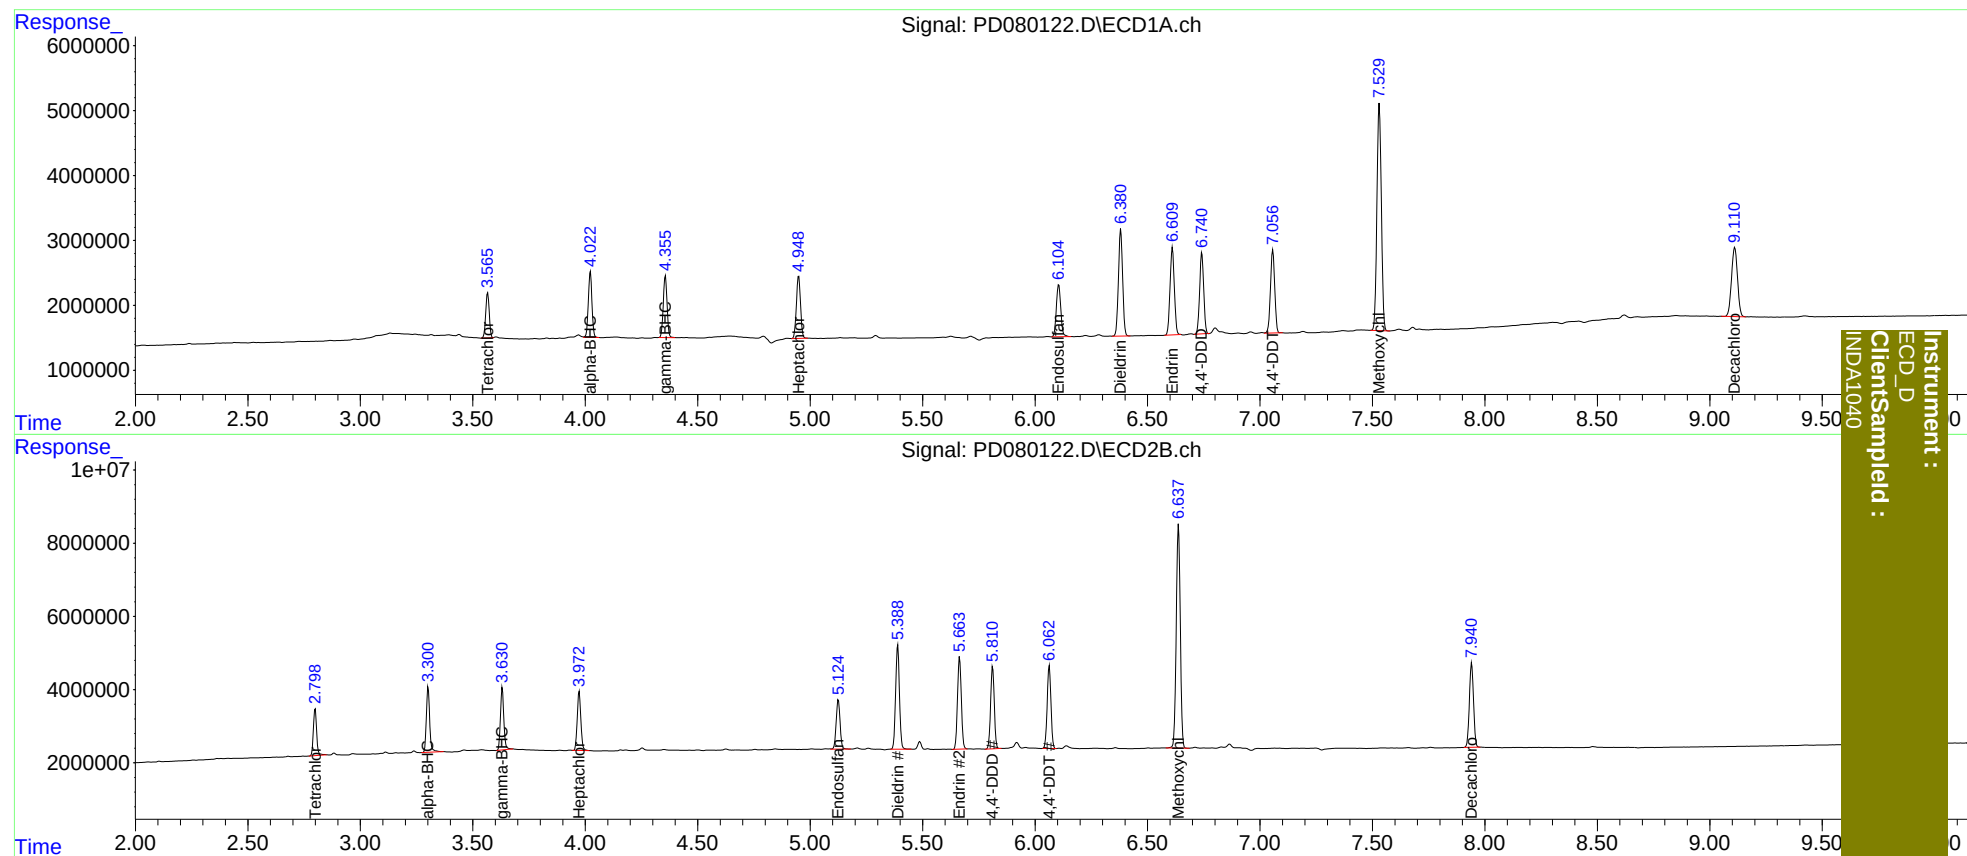

Instrument :
ECD_D
ClientSampled :
INDA1040