

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121723\
 Data File : PD080114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2023 21:03
 Operator : AR\AJ
 Sample : RESC016
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC017

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 02:53:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 02:51:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.800	29575736	50915791	20.746	20.634
2)	SA Decachlor...	9.111	7.941	74526607	111.7E6	41.825	41.201
Target Compounds							
2)	A alpha-BHC	4.023	3.302	23337695	38889134	9.618	9.909
3)	MA gamma-BHC...	4.357	3.632	22649372	36766617	9.804	10.002
4)	MA Heptachlor	4.949	3.973	24411362	37368367	10.190	10.327
5)	MB Aldrin	5.293	4.254	24454607	38875433	11.056	11.153
6)	B beta-BHC	4.550	3.927	11473457	18677560	11.546	10.949
7)	B delta-BHC	4.800	4.157	24568141	40538905	10.638	10.582
8)	B Heptachlo...	5.719	4.755	23242966	36420342	11.110	11.047
9)	A Endosulfan I	6.106	5.125	21684211	32336896	10.608	10.286
10)	B trans-Chl...	5.974	5.006	22175677	35092646	10.968	10.874
11)	B cis-Chlor...	6.055	5.070	22790710	35882067	11.058	10.826
12)	B 4,4'-DDE	6.225	5.259	40295888	65395305	21.000	21.230
13)	MA Dieldrin	6.381	5.390	43133464	70006654	20.059	20.173
14)	MA Endrin	6.611	5.665	36415549	61415244	20.326	20.481
15)	B Endosulfa...	6.829	5.958	41320633	63309155	22.381	21.960
16)	A 4,4'-DDD	6.742	5.812	32164355	53634863	20.068	20.302
17)	MA 4,4'-DDT	7.058	6.063	35355338	55543635	20.546	19.984
18)	B Endrin al...	6.959	6.137	32666310	51394981	22.651	22.906
19)	B Endosulfa...	7.194	6.359	39407299	59935758	22.380	22.204
20)	A Methoxychlor	7.532	6.638	94369407	153.3E6	105.427	110.648
21)	B Endrin ke...	7.680	6.865	43218291	70770104	22.622	22.807

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121723\
Data File : PD080114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 21:03
Operator : AR\AJ
Sample : RESC016
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 02:53:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 02:51:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

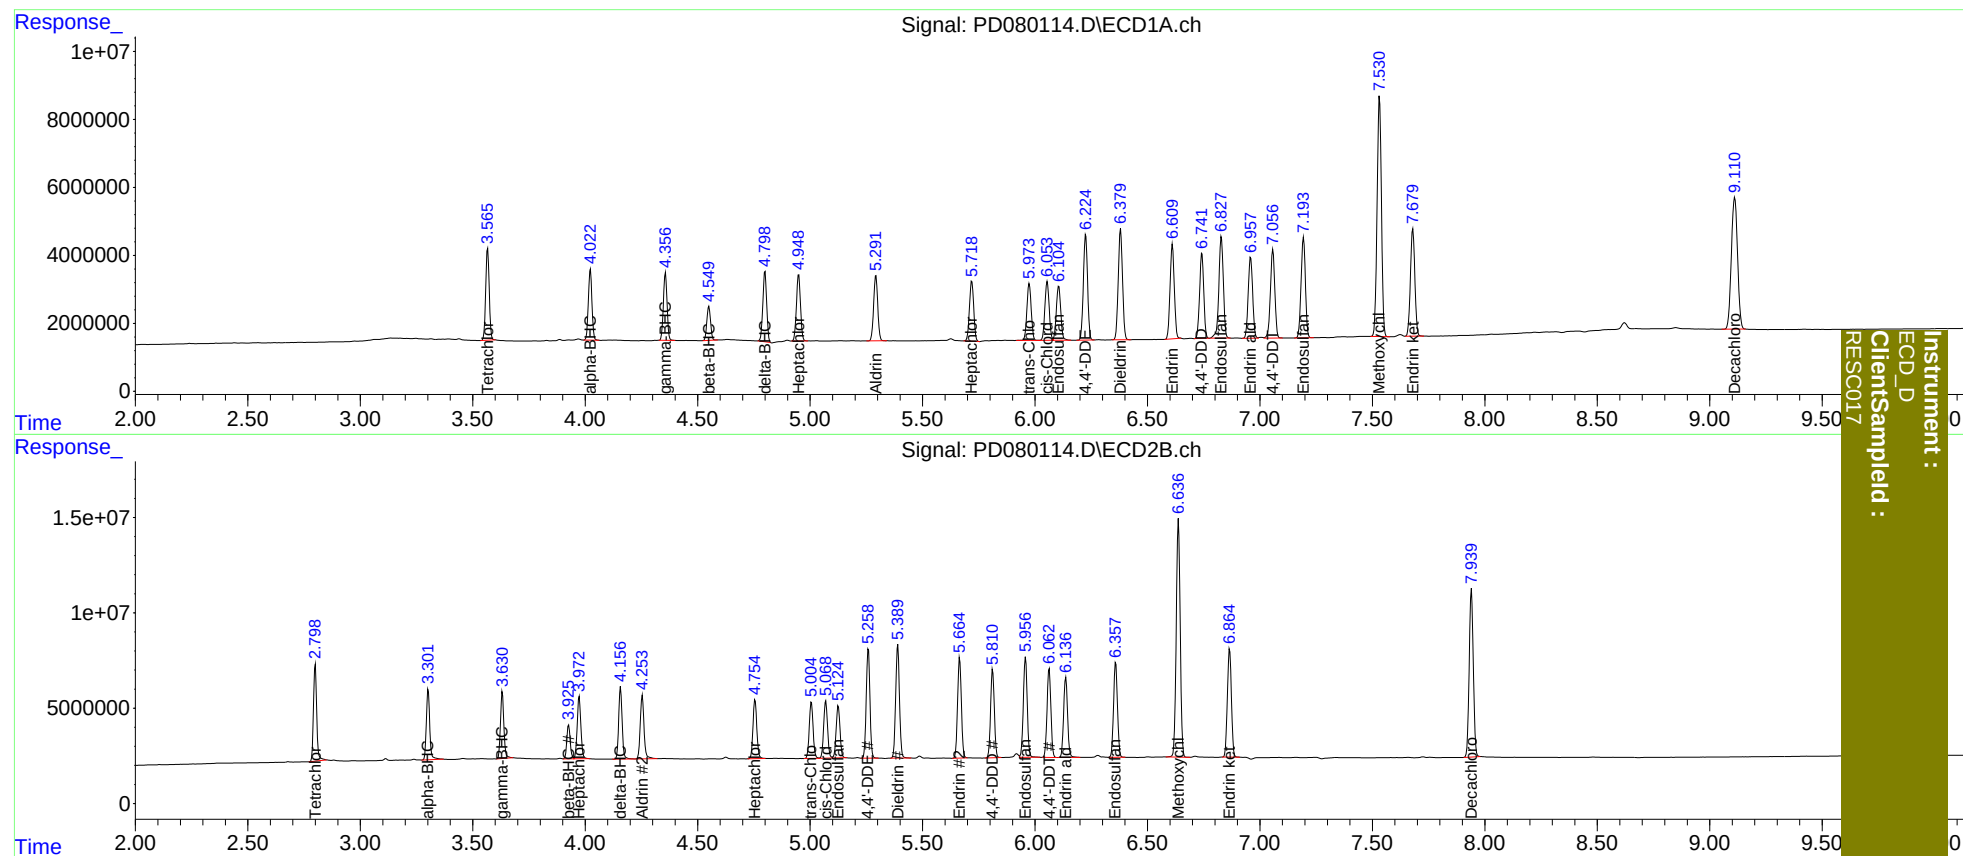

Instrument :
ECD_D
ClientSampled :
RESC017

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121723\
Data File : PD080114.D
Acq On : 15 Dec 2023 21:03
Operator : AR\AJ
Sample : RESC016
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC017

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
Title : GC Extractables
Last Update : Sat Dec 16 02:51:51 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.566	4.023	100.00%
4.023	4.357	100.00%
4.357	4.550	100.00%
4.550	4.800	100.00%
4.800	4.949	100.00%
4.949	5.293	100.00%
5.293	5.719	100.00%
5.719	5.974	100.00%
5.974	6.055	100.00%
6.055	6.106	96.82%
6.106	6.225	100.00%
6.225	6.381	100.00%
6.381	6.611	100.00%
6.611	6.742	100.00%
6.742	6.829	100.00%
6.829	6.959	100.00%
6.959	7.058	100.00%
7.058	7.194	100.00%
7.194	7.532	100.00%
7.532	7.680	100.00%
7.680	9.111	100.00%

Signal #2



2.800	3.302	100.00%
3.302	3.632	100.00%
3.632	3.927	100.00%
3.927	3.973	97.40%
3.973	4.157	100.00%
4.157	4.254	100.00%
4.254	4.755	100.00%
4.755	5.006	100.00%
5.006	5.070	99.06%
5.070	5.125	99.30%
5.125	5.259	100.00%
5.259	5.390	100.00%
5.390	5.665	100.00%
5.665	5.812	100.00%
5.812	5.958	100.00%
5.958	6.063	100.00%
6.063	6.137	100.00%
6.137	6.359	100.00%
6.359	6.638	100.00%
6.638	6.865	100.00%
6.865	7.941	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121723\
Data File : PD080114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 21:03
Operator : AR\AJ
Sample : RESC016
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC017

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 02:53:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 02:51:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

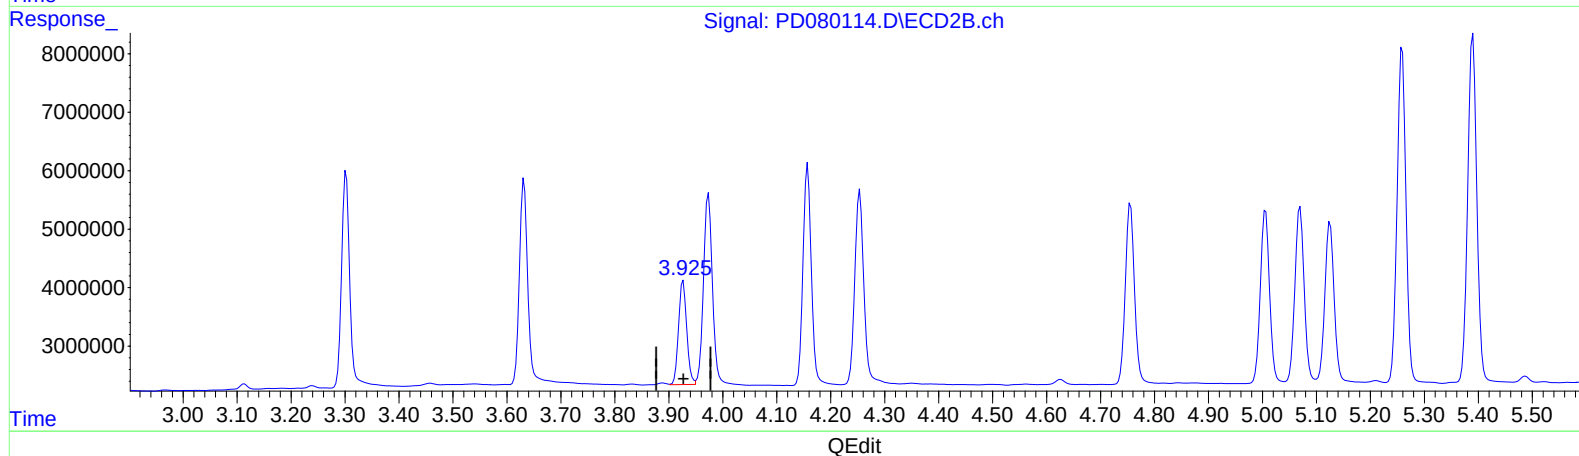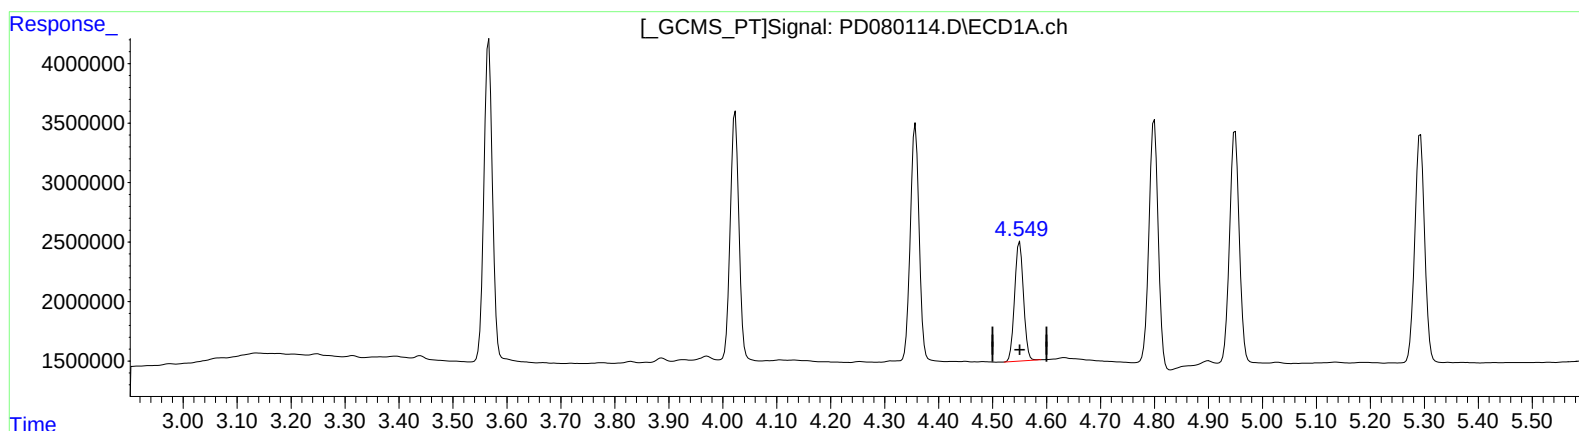

(6) beta-BHC (B)

4.550min 11.546 ng/ml

response 11473457

(6) beta-BHC #2 (B)

3.927min 10.949 ng/ml


response 18677560

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121723\
Data File : PD080114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 21:03
Operator : AR\AJ
Sample : RESC016
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC017

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 02:53:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 02:51:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

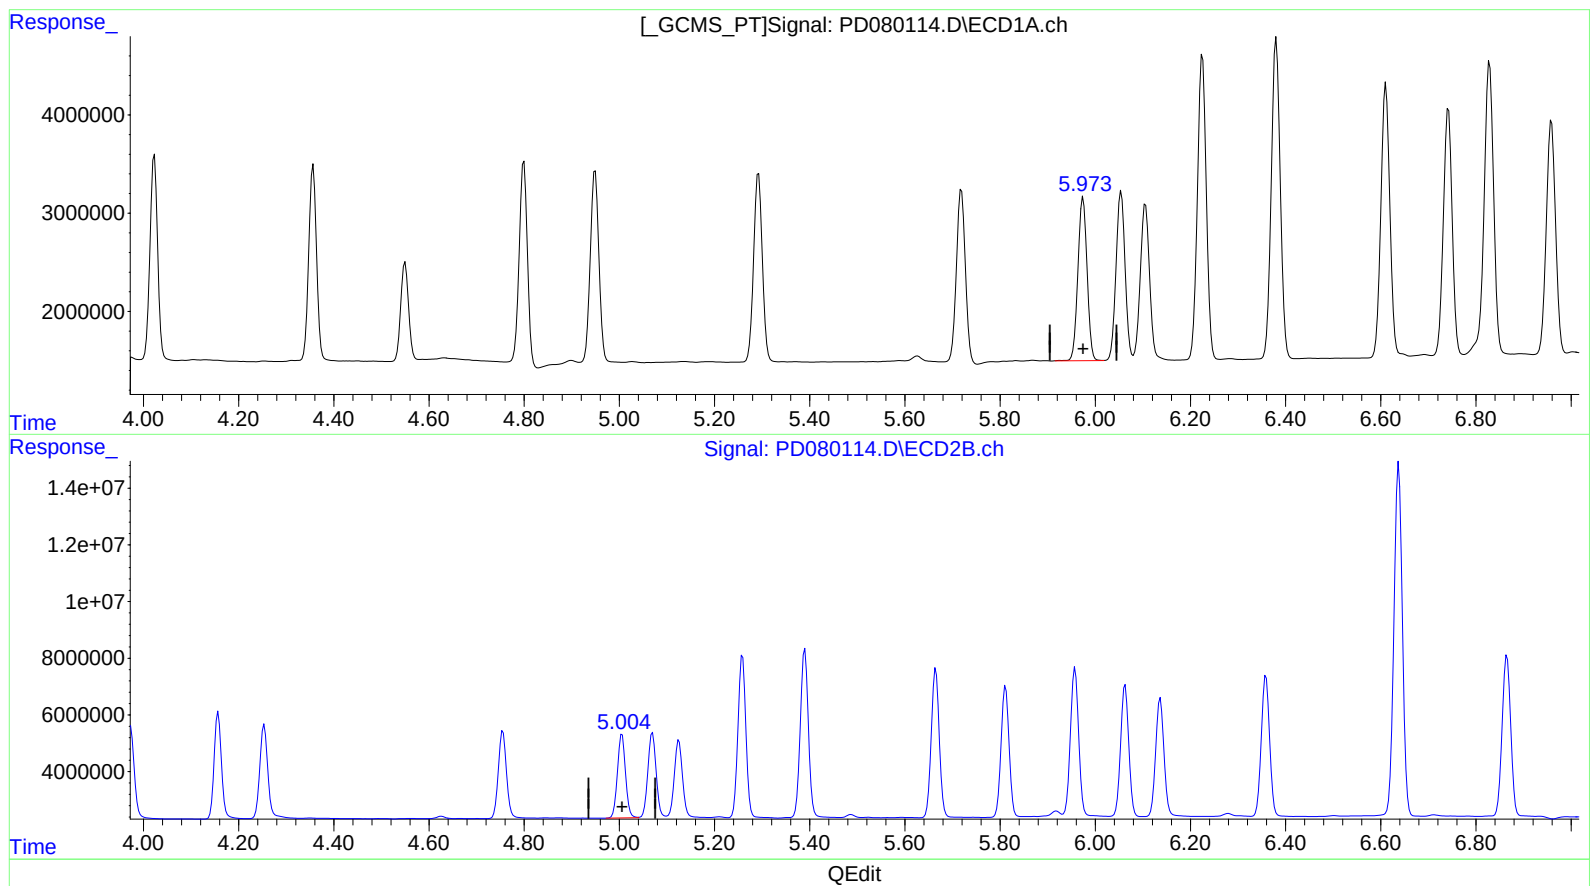

(10) trans-Chlordane (B)

5.974min 10.968 ng/ml

response 22175677

(10) trans-Chlordane #2 (B)

5.006min 10.874 ng/ml


response 35092646

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121723\
Data File : PD080114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 21:03
Operator : AR\AJ
Sample : RESC016
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC017

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 02:53:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 02:51:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

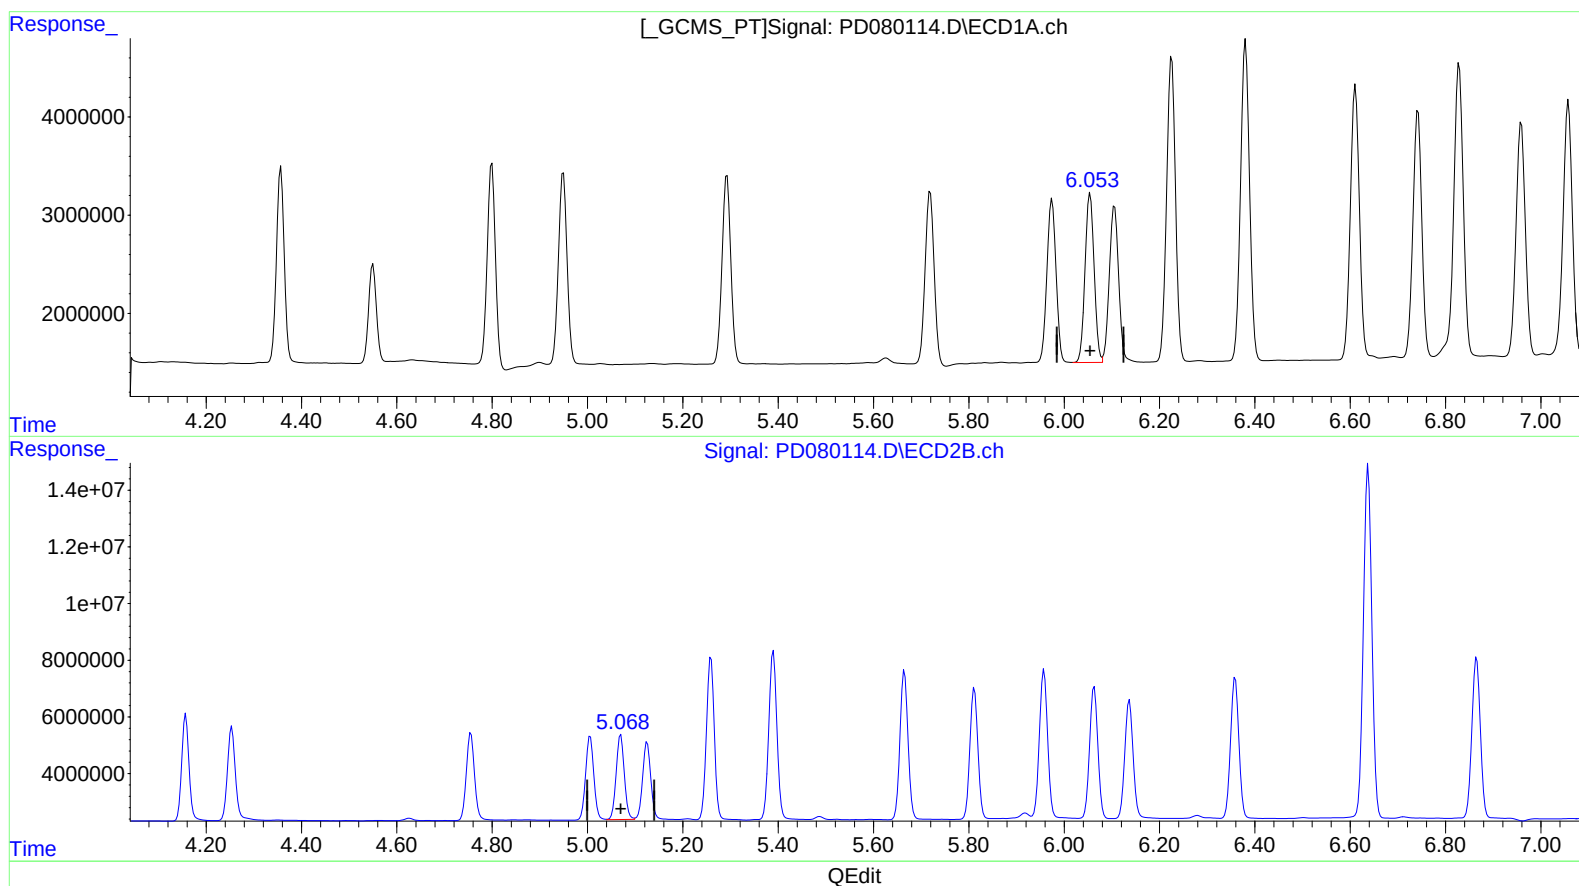

(11) cis-Chlordane (B)

6.055min 11.058 ng/ml

response 22790710

(11) cis-Chlordane #2 (B)

5.070min 10.826 ng/ml

response 35882067