

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121723\
 Data File : PD080133.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2023 01:16
 Operator : AR\AJ
 Sample : INDB601
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDB6051

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/17/2023
 Supervised By : Ankita Jodhani 12/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 02:11:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 02:07:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.799	219.6E6	376.5E6	160.109	159.549
27)	SA Decachlor...	9.111	7.941	517.5E6	809.0E6	307.149	313.143
Target Compounds							
5)	MB Aldrin	5.293	4.254	364.2E6	569.2E6	164.975	163.616
6)	B beta-BHC	4.550	3.926	148.6E6	255.4E6	154.905	155.132
7)	B delta-BHC	4.798	4.157	405.2E6	646.9E6	171.719m	167.095
8)	B Heptachlo...	5.719	4.755	325.9E6	521.9E6	160.056	160.470
10)	B trans-Chl...	5.975	5.006	324.3E6	524.6E6	162.561	163.303
11)	B cis-Chlor...	6.055	5.070	325.1E6	528.6E6	160.738	161.606
12)	B 4,4'-DDE	6.225	5.259	654.5E6	1025.7E6	336.462	329.989
15)	B Endosulfa...	6.829	5.957	568.8E6	901.4E6	318.448	318.199
18)	B Endrin al...	6.959	6.136	441.9E6	685.4E6	315.580	314.152
19)	B Endosulfa...	7.193	6.359	546.6E6	835.3E6	318.182	316.239
21)	B Endrin ke...	7.680	6.865	602.1E6	954.9E6	320.436	314.197

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121723\
Data File : PD080133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2023 01:16
Operator : AR\AJ
Sample : INDB601
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 02:11:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 02:07:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

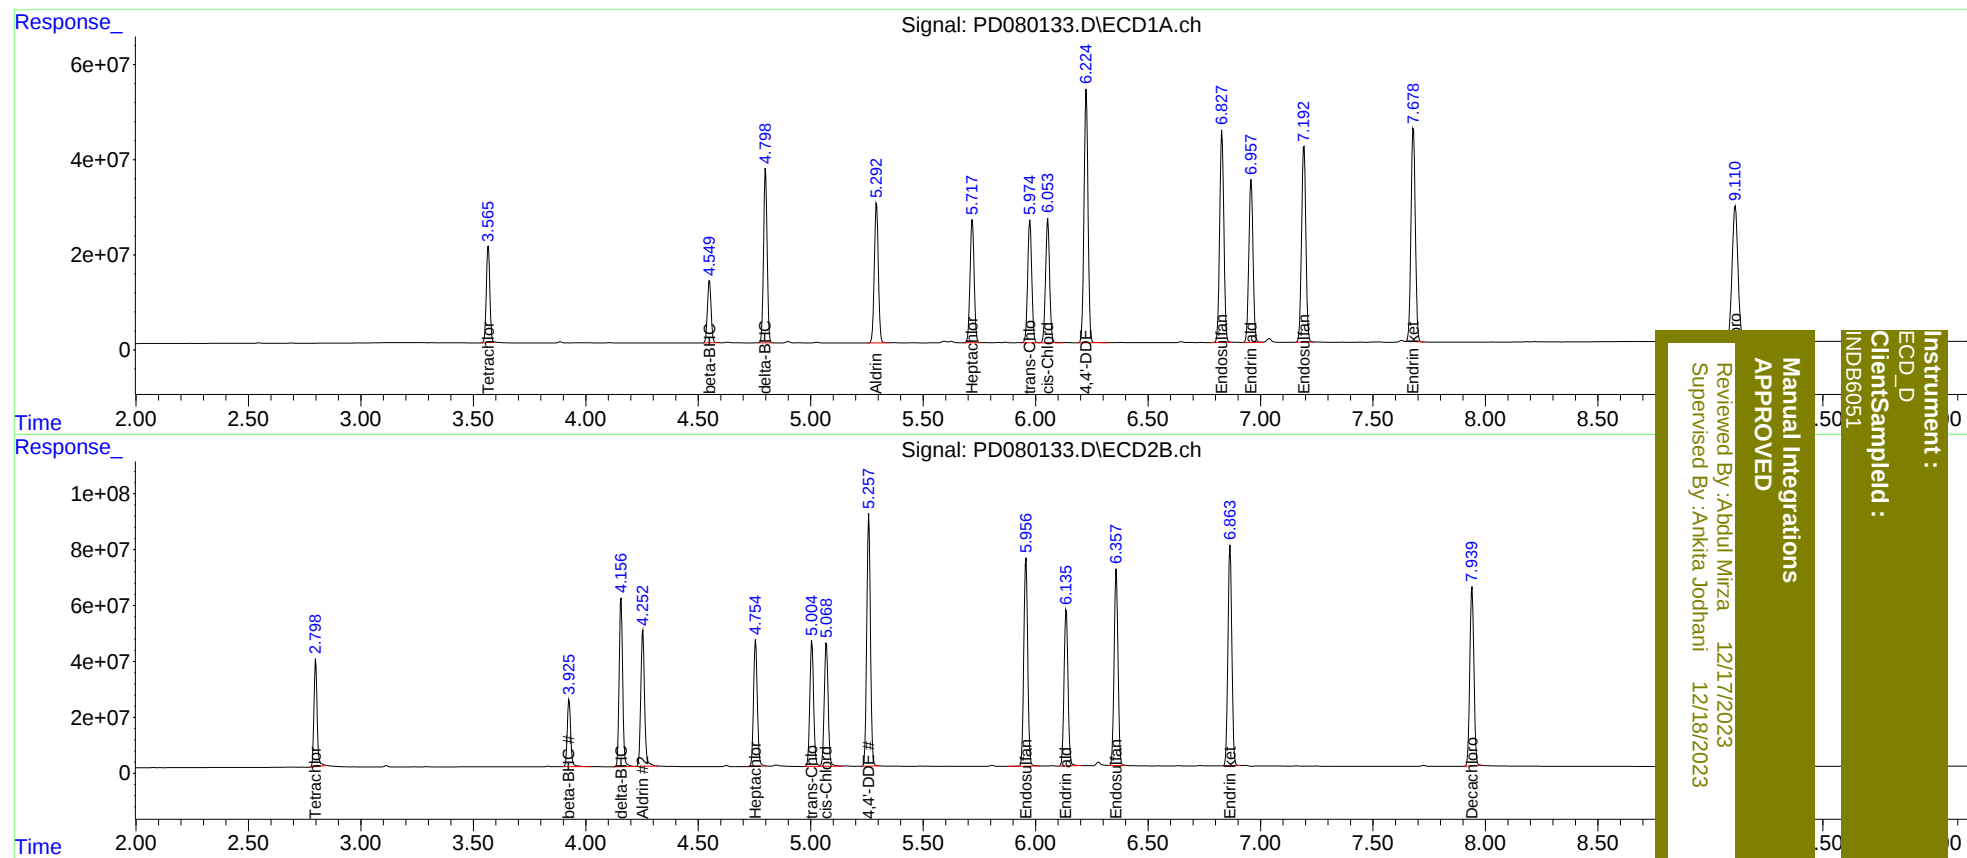

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 12/17/2023
Supervised By: Ankita Jodhani 12/18/2023

Instrument :
ECD_D
Client Sampled :
INDB6051