

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056552.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 14:20
 Operator : SG\AJ
 Sample : K6236-19
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:36:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.961	11375592	20053559	13.735	16.680
27)	SA Decachlor...	7.961	8.999	20195976	26822244	22.366	22.293
Target Compounds							
6)	B beta-BHC	0.000	4.787	0	1004194	N.D.	1.219
15)	B Endosulfa...	0.000	6.875	0	1216982	N.D.	0.831
19)	B Endosulfa...	0.000	7.192	0	191149	N.D.	0.143


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056552.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 14:20
Operator : SG\AJ
Sample : K6236-19
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:36:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

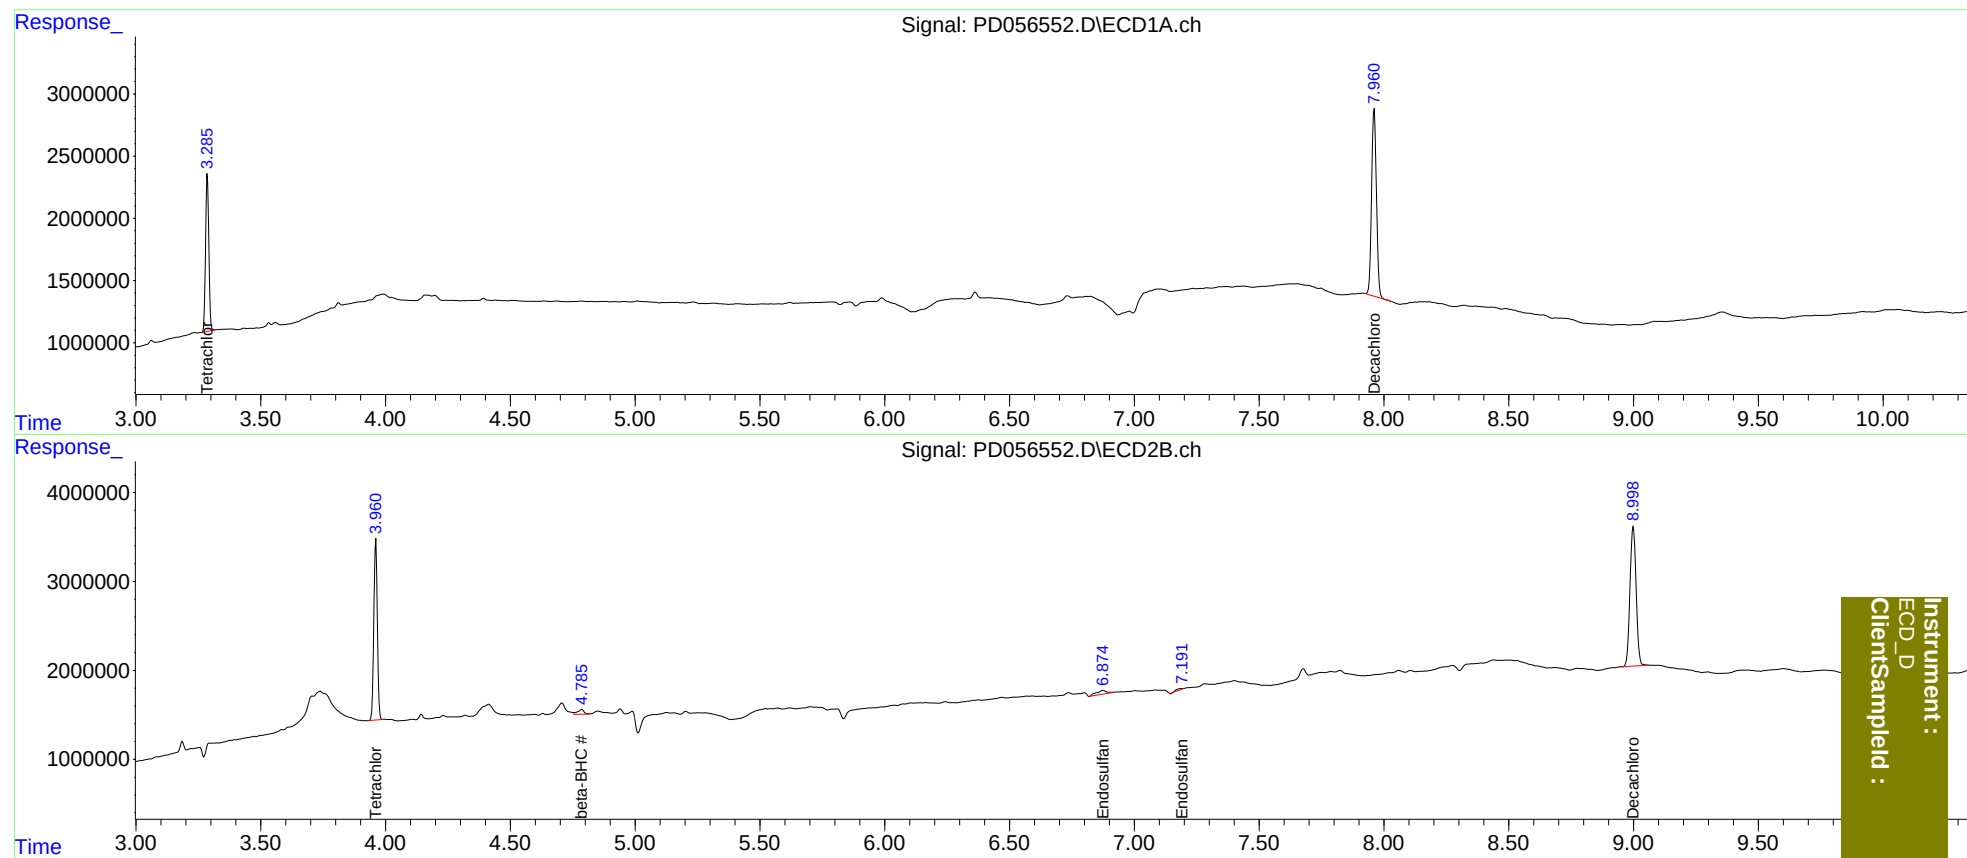


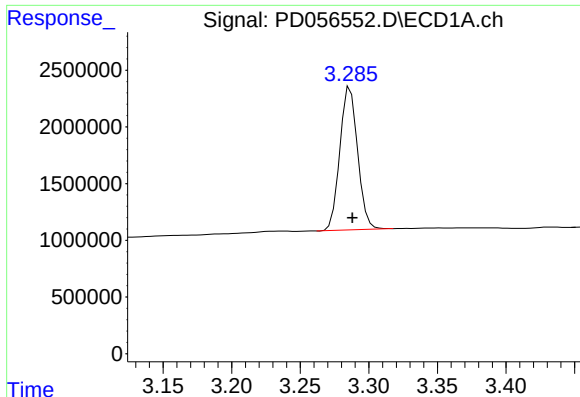

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: -0.001 min
Response: 11375592
Conc: 13.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

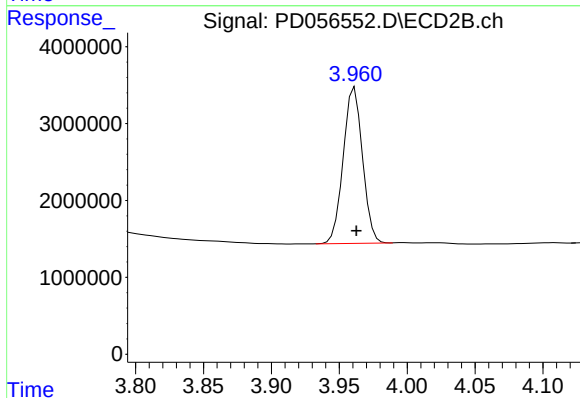


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.001 min
Response: 20053559
Conc: 16.68 ng/ml

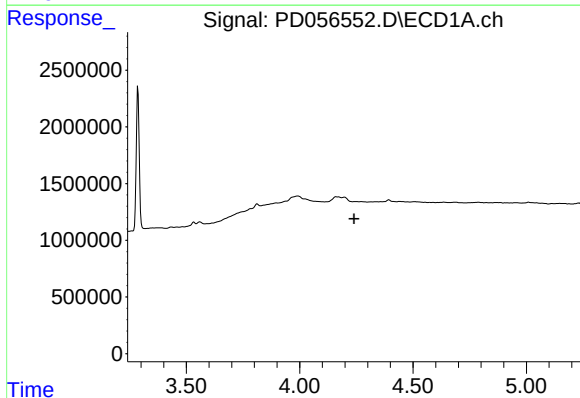


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

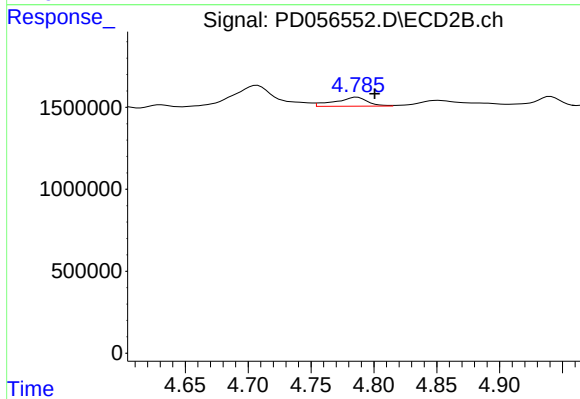

#6 beta-BHC


R.T.: 4.787 min
Delta R.T.: -0.014 min
Response: 1004194
Conc: 1.22 ng/ml

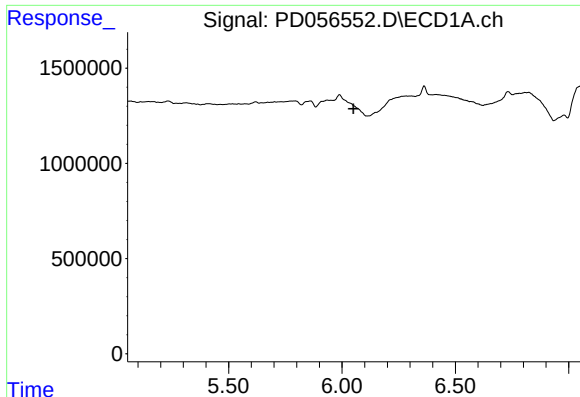

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

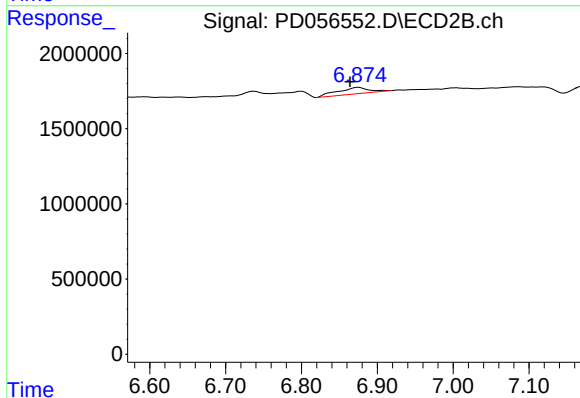


#15 Endosulfan II

R.T.: 6.875 min
Delta R.T.: 0.011 min
Response: 1216982
Conc: 0.83 ng/ml

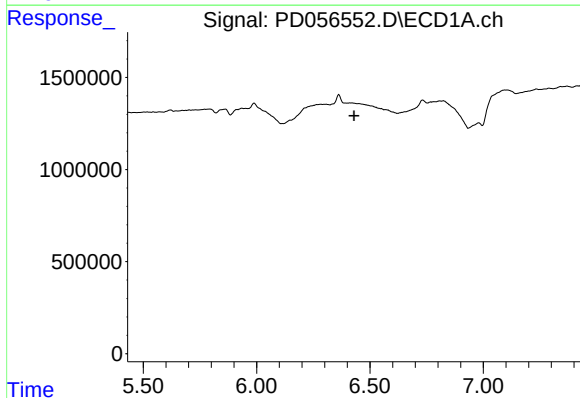


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

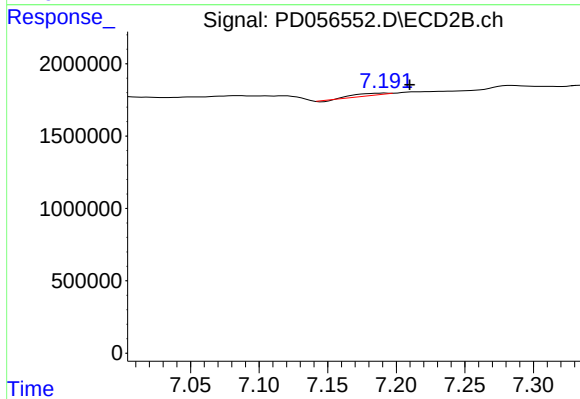

#19 Endosulfan Sulfate


R.T.: 7.192 min
Delta R.T.: -0.018 min
Response: 191149
Conc: 0.14 ng/ml

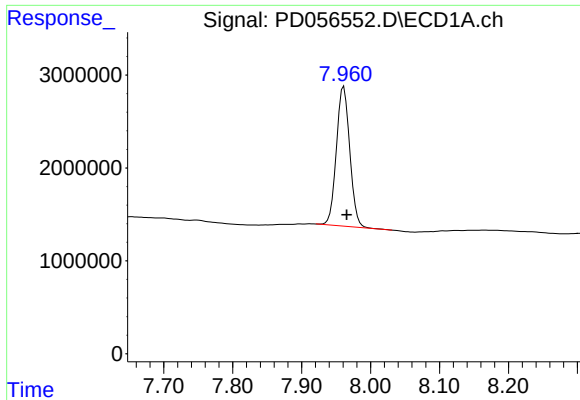

#27 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.004 min
Response: 20195976
Conc: 22.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

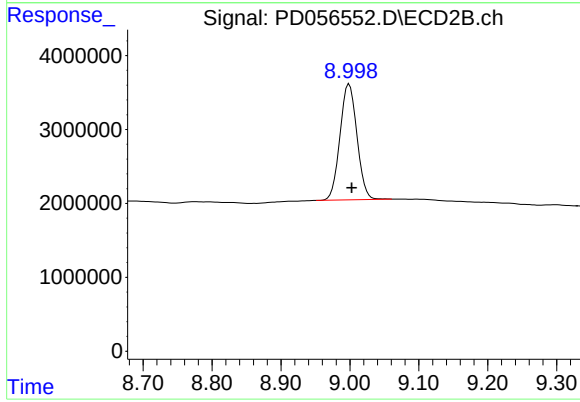

#27 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.004 min
Response: 26822244
Conc: 22.29 ng/ml