

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 17:30
 Operator : SG\AJ
 Sample : PB125535BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:43:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.293	3.960	20383087	30747312	24.611	25.575
2)	SA Decachlor...	7.970	9.001	34140306	50239028	37.809	41.756
Target Compounds							
3)	MA gamma-BHC...	3.972	0.000	1332910	0	1.187	N.D. #
14)	MA Endrin	0.000	6.724f	0	890330	N.D.	0.703
15)	B Endosulfa...	0.000	6.871	0	745846	N.D.	0.509
16)	A 4,4'-DDD	0.000	6.724f	0	890330	N.D.	0.757

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 17:30
Operator : SG\AJ
Sample : PB125535BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:43:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

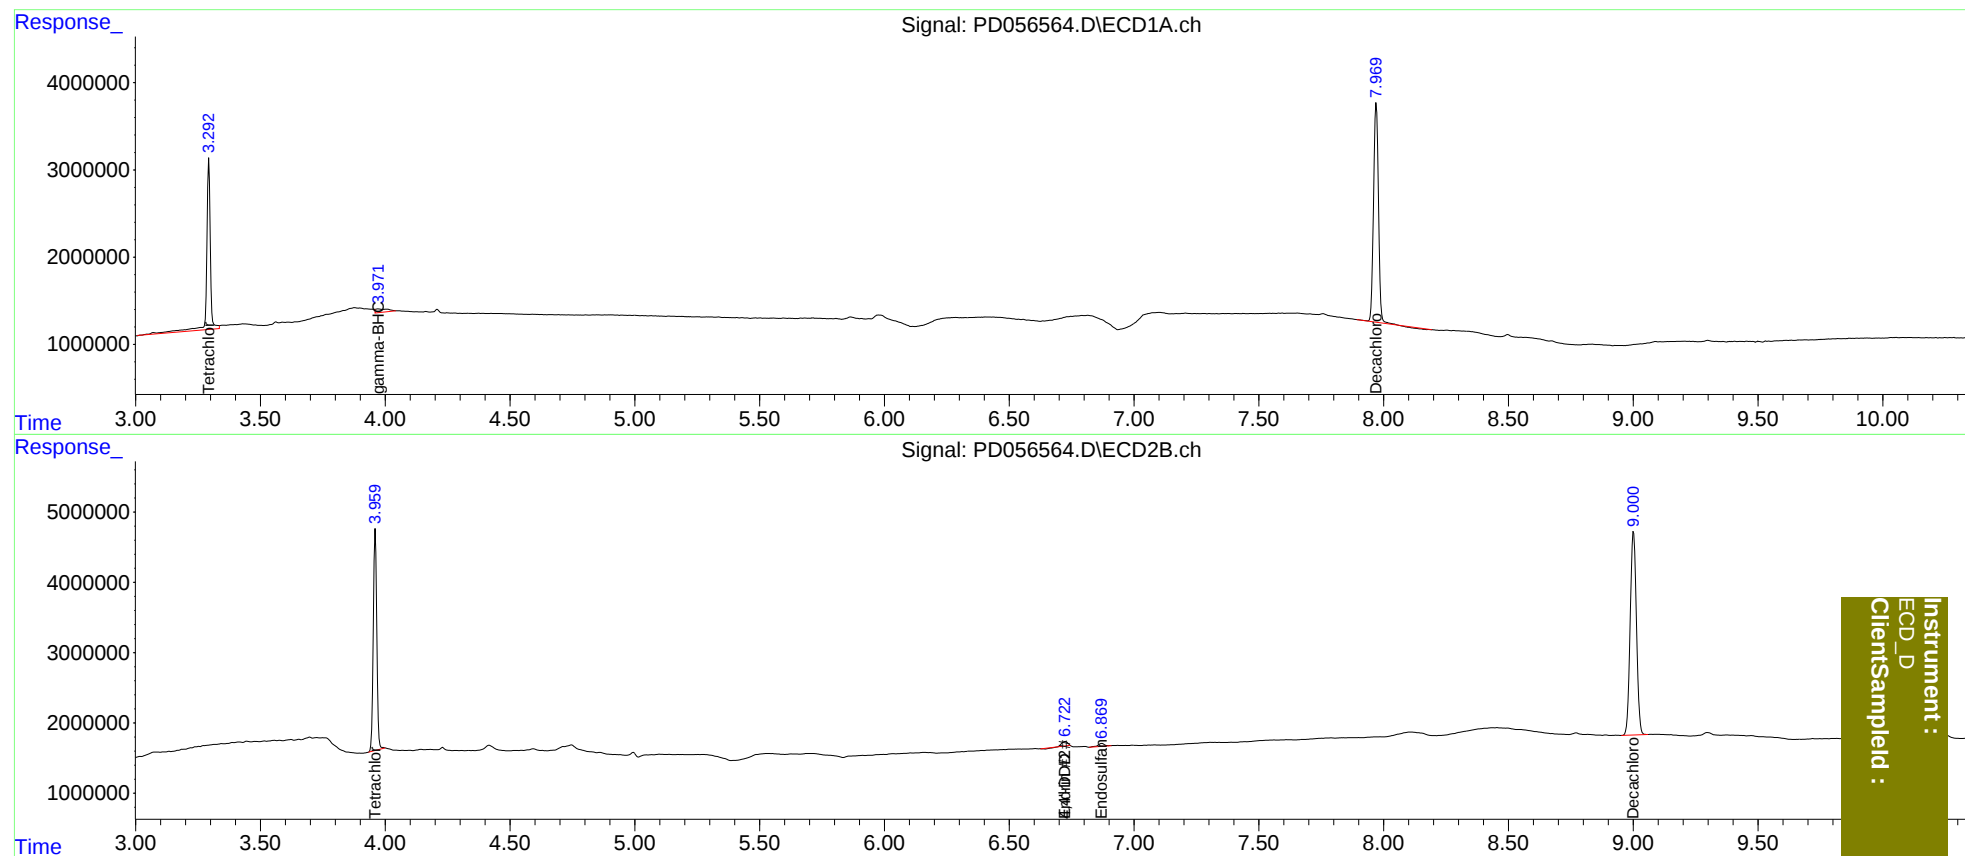

Instrument :
ECD_D
ClientSampleId :

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :