

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 18:25
 Operator : SG\AJ
 Sample : K6276-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:43:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.960	18036199	32481955	21.778	27.018
27)	SA Decachlor...	7.971	9.001	27394543	37986328	30.338	31.572
Target Compounds							
3)	MA gamma-BHC...	4.007	4.638	3516755	617914	3.132	0.383 #
4)	MA Heptachlor	0.000	5.157	0	614412	N.D.	0.377
6)	B beta-BHC	0.000	4.794	0	1357681	N.D.	1.647
7)	B delta-BHC	0.000	4.990f	0	5000126	N.D.	3.002
8)	B Heptachlo...	0.000	5.789f	0	6621176	N.D.	4.274
14)	MA Endrin	0.000	6.721f	0	974972	N.D.	0.770
15)	B Endosulfa...	0.000	6.872	0	1276789	N.D.	0.871
16)	A 4,4'-DDD	0.000	6.721f	0	974972	N.D.	0.829

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 18:25
Operator : SG\AJ
Sample : K6276-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:43:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

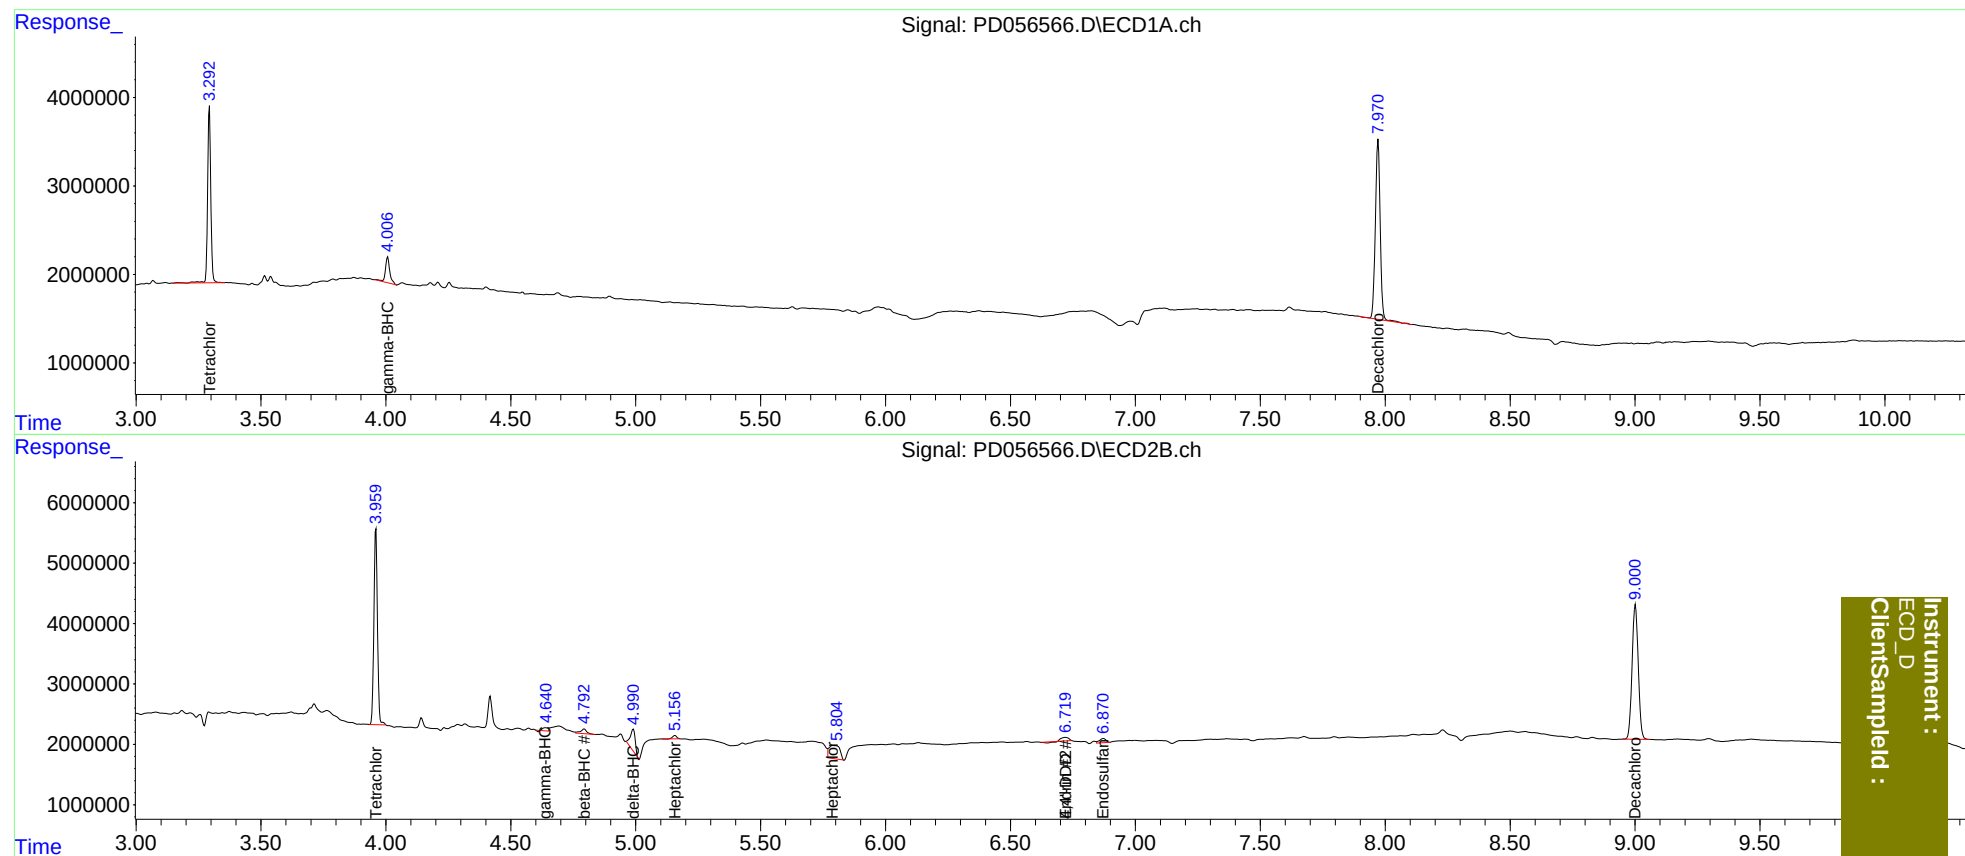

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :