

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 18:39
 Operator : SG\AJ
 Sample : K6276-02
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:43:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.961	15867805	26505910	19.159	22.047
27)	SA Decachlor...	7.962	8.997	22608961	32166297	25.038	26.735
Target Compounds							
2)	A alpha-BHC	3.667f	0.000	926689	0	0.787	N.D. #
3)	MA gamma-BHC...	3.999	4.594f	3382584	622674	3.012	0.386 #
5)	MB Aldrin	0.000	5.485f	0	2036491	N.D.	1.239
6)	B beta-BHC	0.000	4.795	0	3316193	N.D.	4.024
7)	B delta-BHC	0.000	4.988f	0	3297618	N.D.	1.980
8)	B Heptachlo...	0.000	5.811	0	4025228	N.D.	2.598
9)	A Endosulfan I	0.000	6.131f	0	527989	N.D.	0.364
10)	B trans-Chl...	0.000	6.060	0	2738363	N.D.	1.656
11)	B cis-Chlor...	0.000	6.131	0	527989	N.D.	0.328
13)	MA Dieldrin	0.000	6.380f	0	1207982	N.D.	0.769
15)	B Endosulfa...	6.007f	6.828f	6643917	829588	6.975	0.566 #
16)	A 4,4'-DDD	0.000	6.828f	0	829588	N.D.	0.705
17)	MA 4,4'-DDT	6.205f	7.113f	1465175	2286453	2.082	1.934
18)	B Endrin al...	6.205	0.000	1465175	0	1.843	N.D. #
19)	B Endosulfa...	0.000	7.216	0	1213510	N.D.	0.908
21)	B Endrin ke...	0.000	7.641f	0	740915	N.D.	0.504
22)	Toxaphene-1	0.000	6.380	0	1207982	N.D.	107.597
23)	Toxaphene-2	5.619	6.584	1263381	539519	129.830	39.095 #
24)	Toxaphene-3	6.007	0.000	6643917	0	802.881	N.D. #
25)	Toxaphene-4	0.000	7.113	0	2286453	N.D.	41.410
26)	Toxaphene-5	0.000	7.641	0	740915	N.D.	28.988

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 18:39
Operator : SG\AJ
Sample : K6276-02
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:43:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

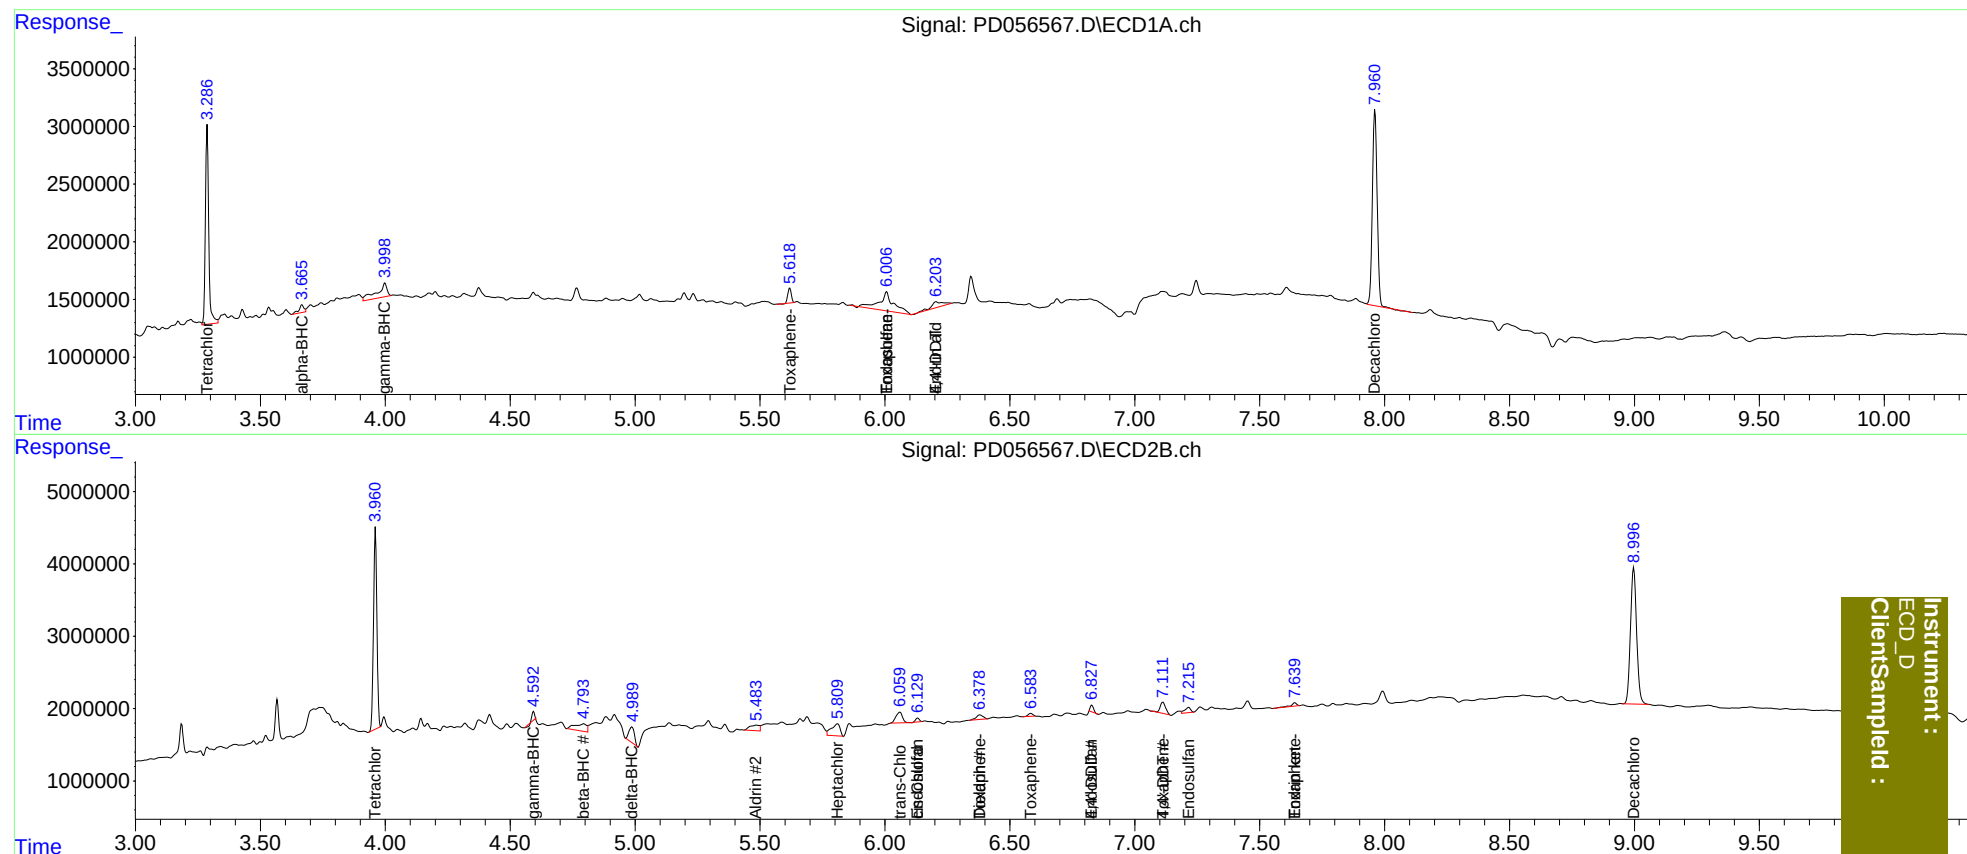

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :