

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 19:35
 Operator : SG\AJ
 Sample : K6276-06
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:44:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.962	17435739	28217380	21.053	23.470
2)	SA Decachlor...	7.961	8.998	24373730	34572170	26.993	28.735
Target Compounds							
2)	A alpha-BHC	3.703	4.389f	2181889	1490732	1.853	0.894 #
3)	MA gamma-BHC...	3.999	4.596f	10152577	295505	9.041	0.183 #
5)	MB Aldrin	0.000	5.435	0	1200406	N.D.	0.731
6)	B beta-BHC	0.000	4.791	0	1039635	N.D.	1.262
7)	B delta-BHC	0.000	5.055f	0	2409141	N.D.	1.446
8)	B Heptachlo...	0.000	5.858	0	916860	N.D.	0.592
9)	A Endosulfan I	5.295	0.000	1669911	0	1.806	N.D. #
10)	B trans-Chl...	0.000	6.045	0	2628239	N.D.	1.590
11)	B cis-Chlor...	5.295f	0.000	1669911	0	1.635	N.D. #
16)	A 4,4'-DDD	0.000	6.731f	0	1165747	N.D.	0.991
18)	B Endrin al...	6.228	0.000	13570	0	<MDL	N.D. #
19)	B Endosulfa...	6.498f	7.199	5599404	9029081	6.446	6.753
20)	A Methoxychlor	6.701	0.000	1877351	0	5.539	N.D. #
21)	B Endrin ke...	0.000	7.637f	0	4644220	N.D.	3.156
23)	Toxaphene-2	0.000	6.581	0	1303979	N.D.	94.489
26)	Toxaphene-5	0.000	7.637	0	4644220	N.D.	181.706

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 19:35
Operator : SG\AJ
Sample : K6276-06
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:44:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

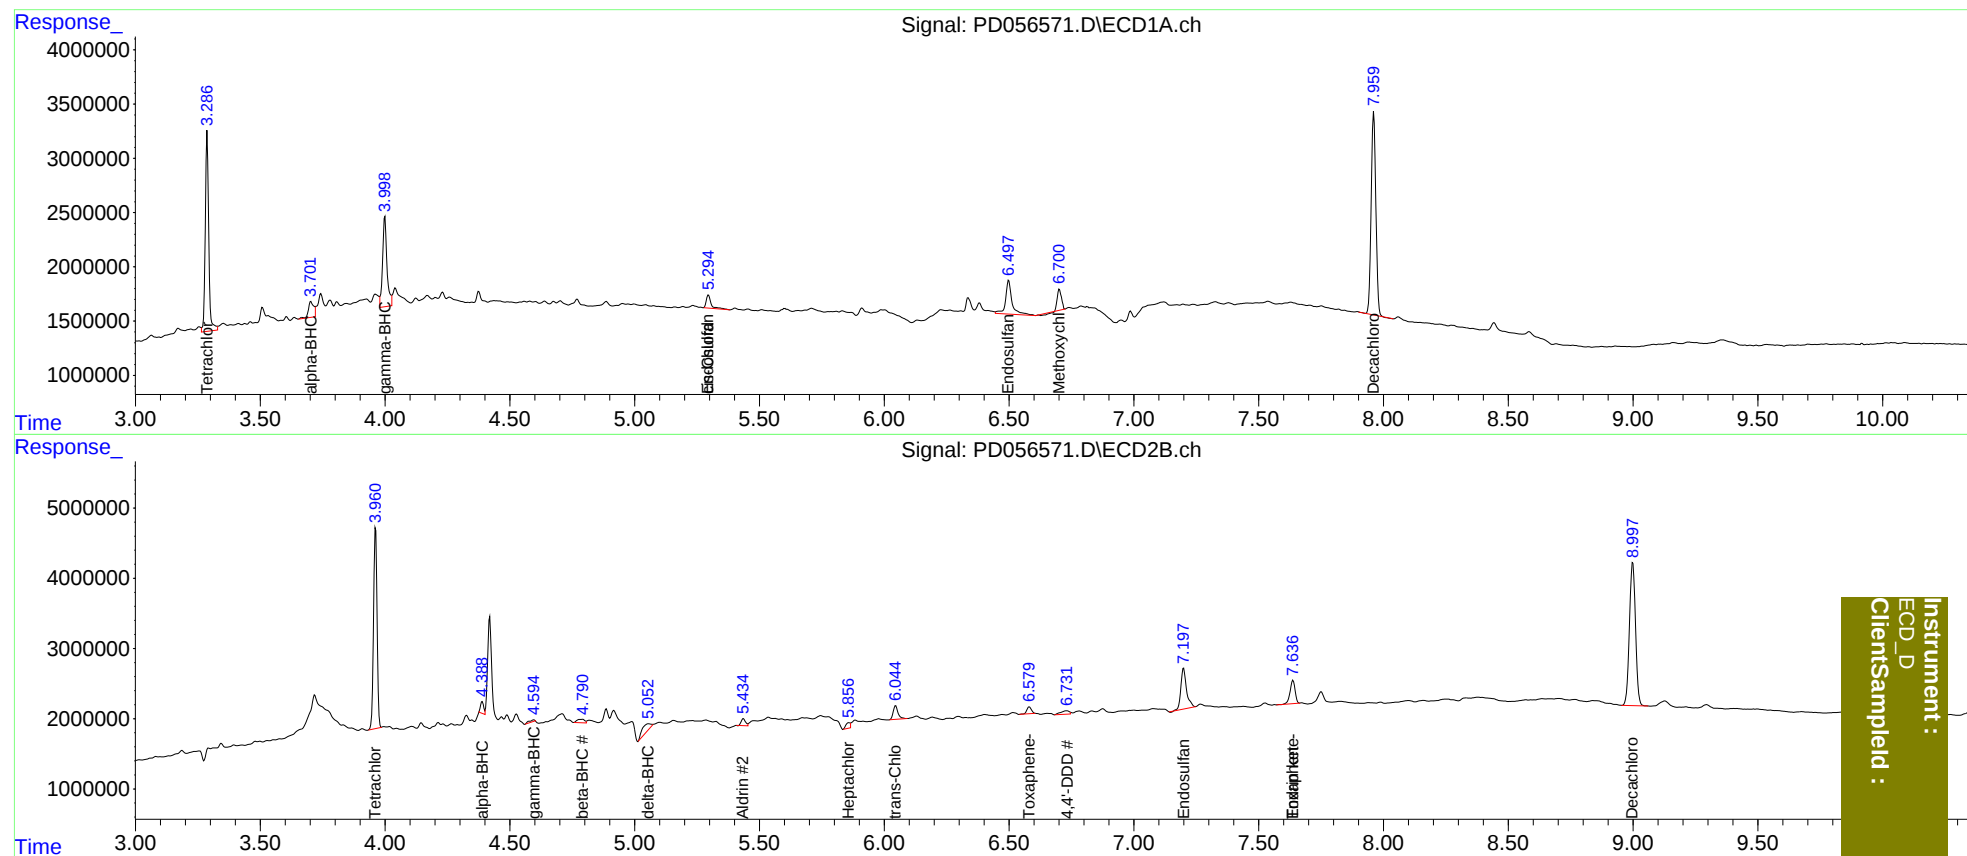

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :