

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 19:49
 Operator : SG\AJ
 Sample : K6276-07
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:44:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.962	21623122	31792850	26.109	26.444
27)	SA Decachlor...	7.960	8.998	27946334	38832858	30.949	32.276
Target Compounds							
2)	A alpha-BHC	3.702	4.388f	2122079	654161	1.802	0.392 #
3)	MA gamma-BHC...	3.998	0.000	8827328	0	7.861	N.D. #
8)	B Heptachlo...	0.000	5.892f	0	2301211	N.D.	1.485
15)	B Endosulfa...	6.005f	6.828f	10980359	2636620	11.527	1.799 #
16)	A 4,4'-DDD	0.000	6.828f	0	2636620	N.D.	2.241
18)	B Endrin al...	6.231	0.000	243028	0	0.306	N.D. #
19)	B Endosulfa...	0.000	7.192	0	905520	N.D.	0.677
24)	Toxaphene-3	6.005	0.000	10980359	0	1326.916	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 19:49
Operator : SG\AJ
Sample : K6276-07
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:44:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

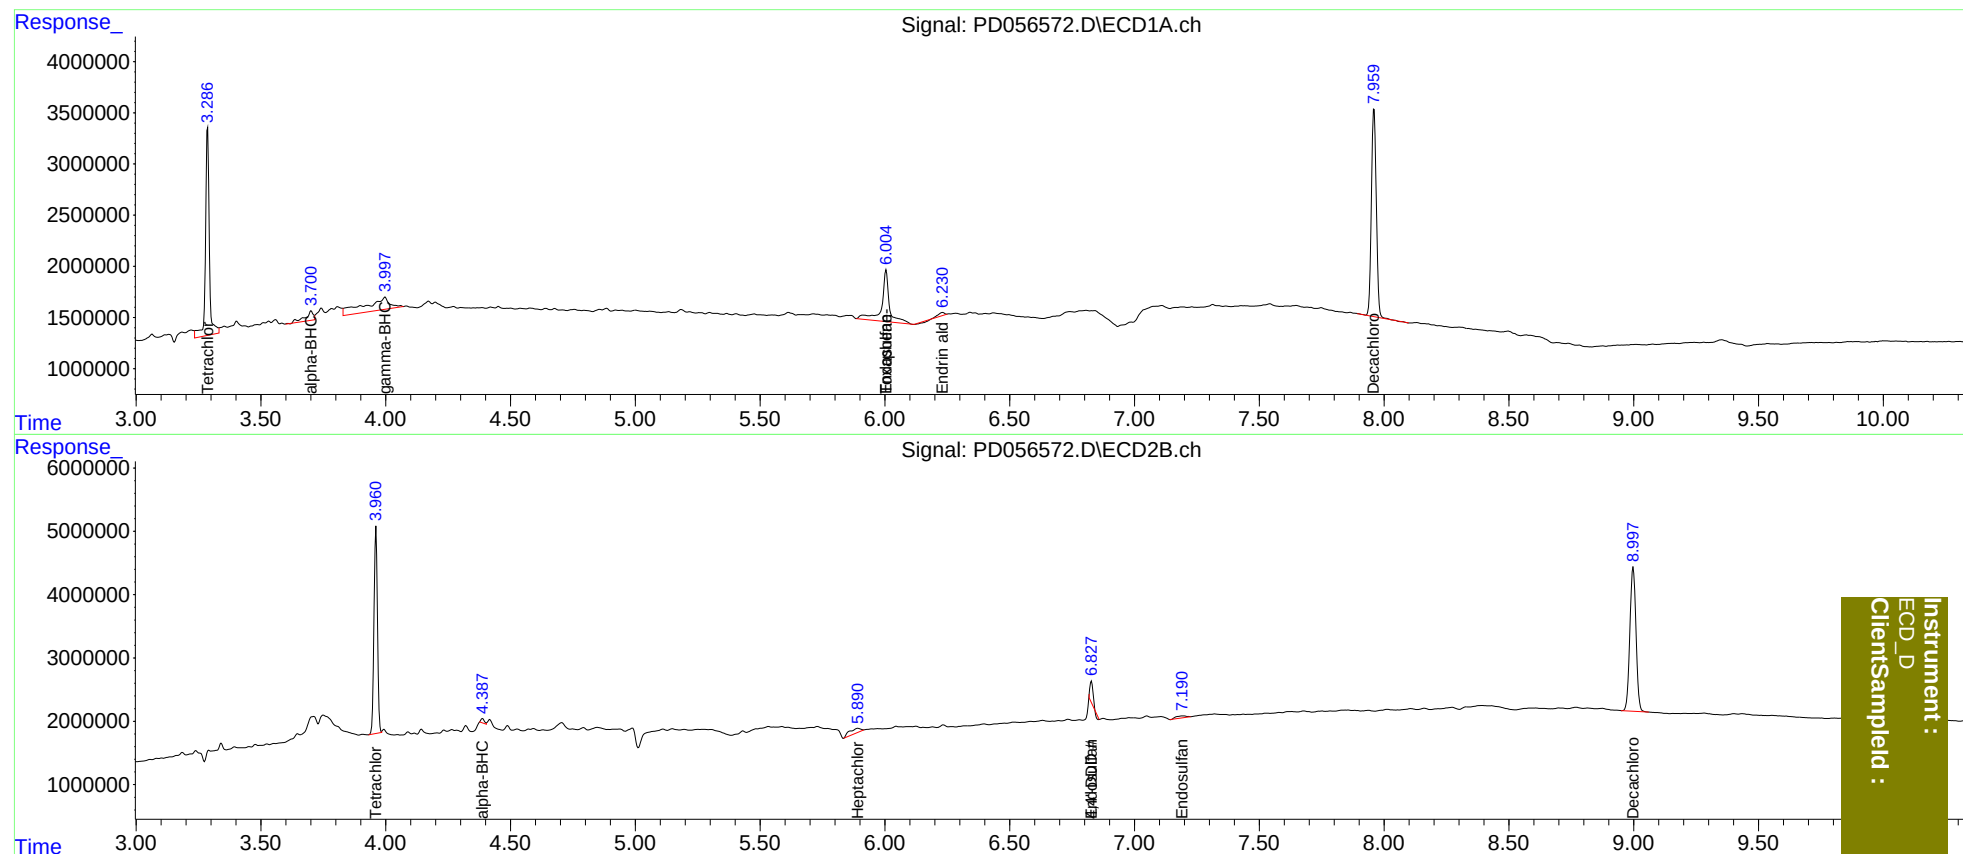

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :