

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 20:17
 Operator : SG\AJ
 Sample : K6276-15
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:44:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.962	17181890	28833308	20.746	23.983
27)	SA Decachlor...	7.960	8.998	21175181	29223203	23.451	24.289
Target Compounds							
3)	MA gamma-BHC...	3.999	4.633	6913565	116241	6.157	<MDL #
6)	B beta-BHC	0.000	4.794	0	225987	N.D.	0.274
7)	B delta-BHC	0.000	4.989f	0	4074259	N.D.	2.446
9)	A Endosulfan I	0.000	6.215	0	708282	N.D.	0.488
10)	B trans-Chl...	0.000	6.047	0	960722	N.D.	0.581
16)	A 4,4'-DDD	0.000	6.734f	0	973686	N.D.	0.827
19)	B Endosulfa...	6.421	7.210	1365456	731112	1.572	0.547 #
21)	B Endrin ke...	0.000	7.641f	0	656085	N.D.	0.446
23)	Toxaphene-2	5.618	0.000	1888433	0	194.063	N.D. #
26)	Toxaphene-5	0.000	7.641	0	656085	N.D.	25.669

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 20:17
Operator : SG\AJ
Sample : K6276-15
Misc :
ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:44:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

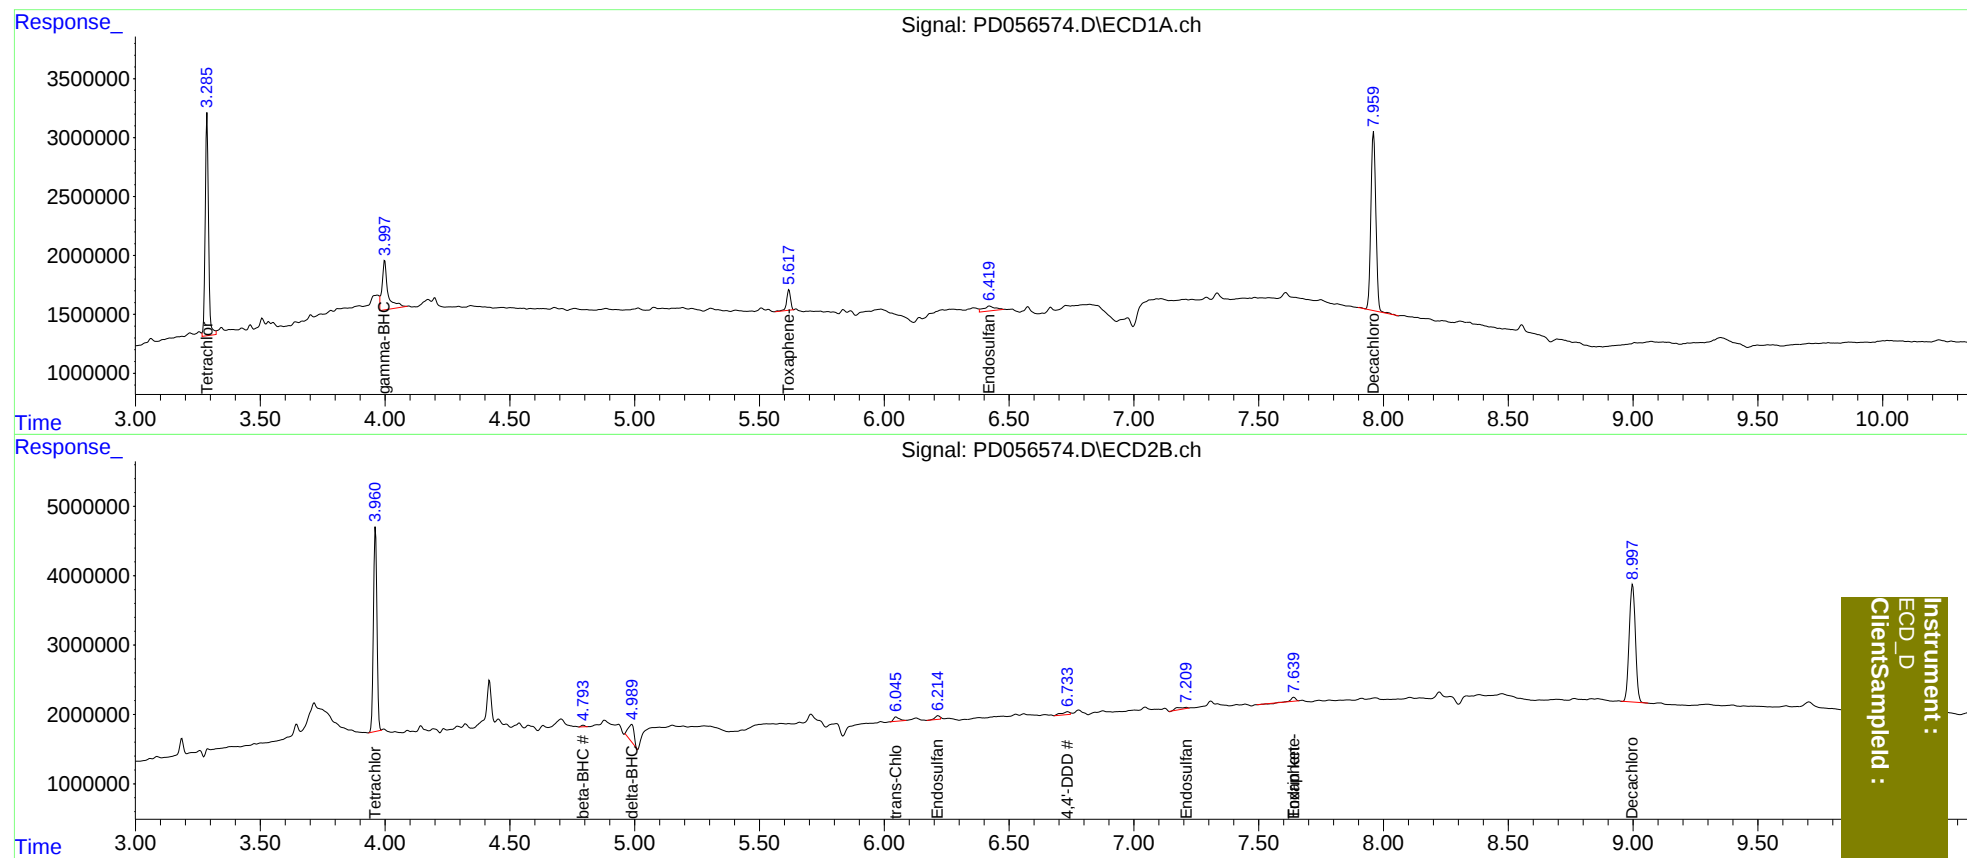

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :