

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 20:45
 Operator : SG\AJ
 Sample : K6276-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:45:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.961	16916771	29605684	20.426	24.625
27)	SA Decachlor...	7.960	8.998	28488737	38464900	31.550	31.970
Target Compounds							
2)	A alpha-BHC	3.702	0.000	1713937	0	1.456	N.D. #
3)	MA gamma-BHC...	3.999	0.000	21344812	0	19.008	N.D. #
6)	B beta-BHC	4.200f	0.000	1185792	0	2.203	N.D. #
7)	B delta-BHC	0.000	4.989f	0	2836092	N.D.	1.703
8)	B Heptachlo...	0.000	5.812	0	2526789	N.D.	1.631
10)	B trans-Chl...	0.000	5.997f	0	2056173	N.D.	1.244
16)	A 4,4'-DDD	0.000	6.734f	0	1081176	N.D.	0.919
19)	B Endosulfa...	6.416	7.198	11935532	2437215	13.741	1.823 #
21)	B Endrin ke...	0.000	7.636f	0	1356762	N.D.	0.922
26)	Toxaphene-5	0.000	7.636	0	1356762	N.D.	53.084

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 20:45
Operator : SG\AJ
Sample : K6276-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:45:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

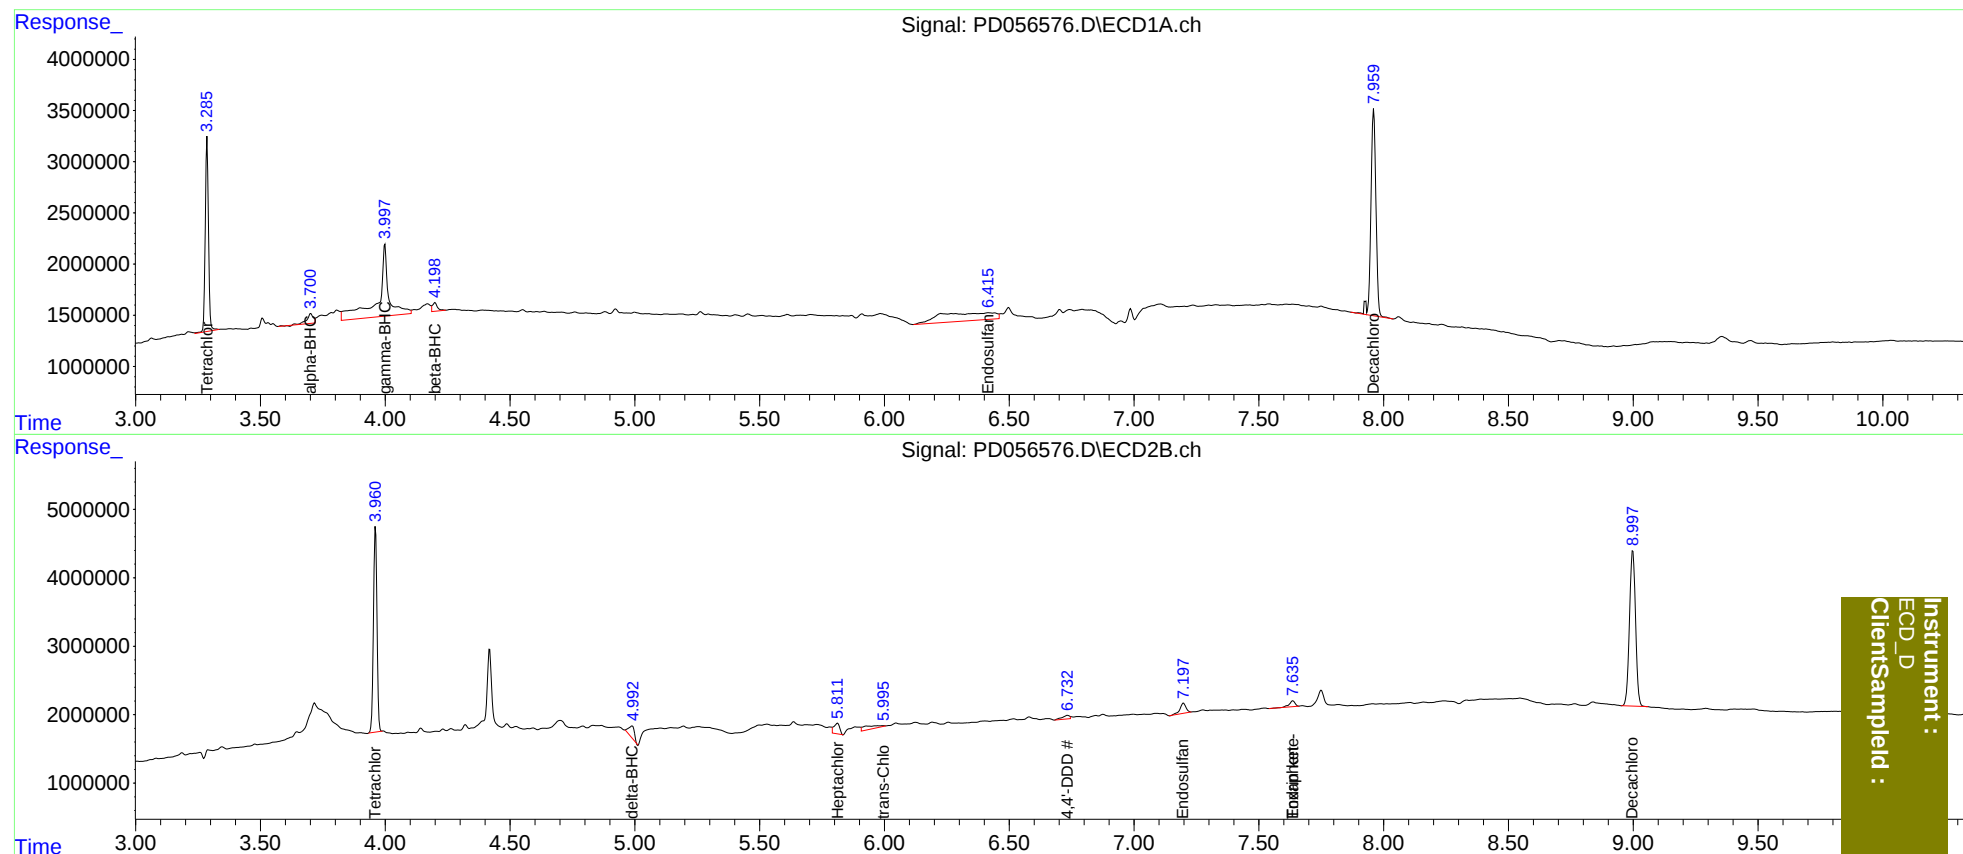

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :