

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 21:27
 Operator : SG\AJ
 Sample : K6276-20
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:45:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.962	19551048	30905635	23.607	25.706
27)	SA Decachlor...	7.960	8.998	27311775	38376282	30.247	31.897
Target Compounds							
3)	MA gamma-BHC...	3.999	0.000	21994404	0	19.586	N.D. #
6)	B beta-BHC	4.200f	4.795	1024902	643342	1.904	0.781 #
7)	B delta-BHC	0.000	4.989f	0	3485858	N.D.	2.093
8)	B Heptachlo...	0.000	5.807	0	5284698	N.D.	3.411
10)	B trans-Chl...	0.000	6.044	0	674379	N.D.	0.408
15)	B Endosulfa...	0.000	6.875	0	1264067	N.D.	0.863
16)	A 4,4'-DDD	0.000	6.735f	0	969450	N.D.	0.824
18)	B Endrin al...	6.264f	0.000	7102175	0	8.935	N.D. #
19)	B Endosulfa...	6.498f	7.199	9903640	1846225	11.402	1.381 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 21:27
Operator : SG\AJ
Sample : K6276-20
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:45:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

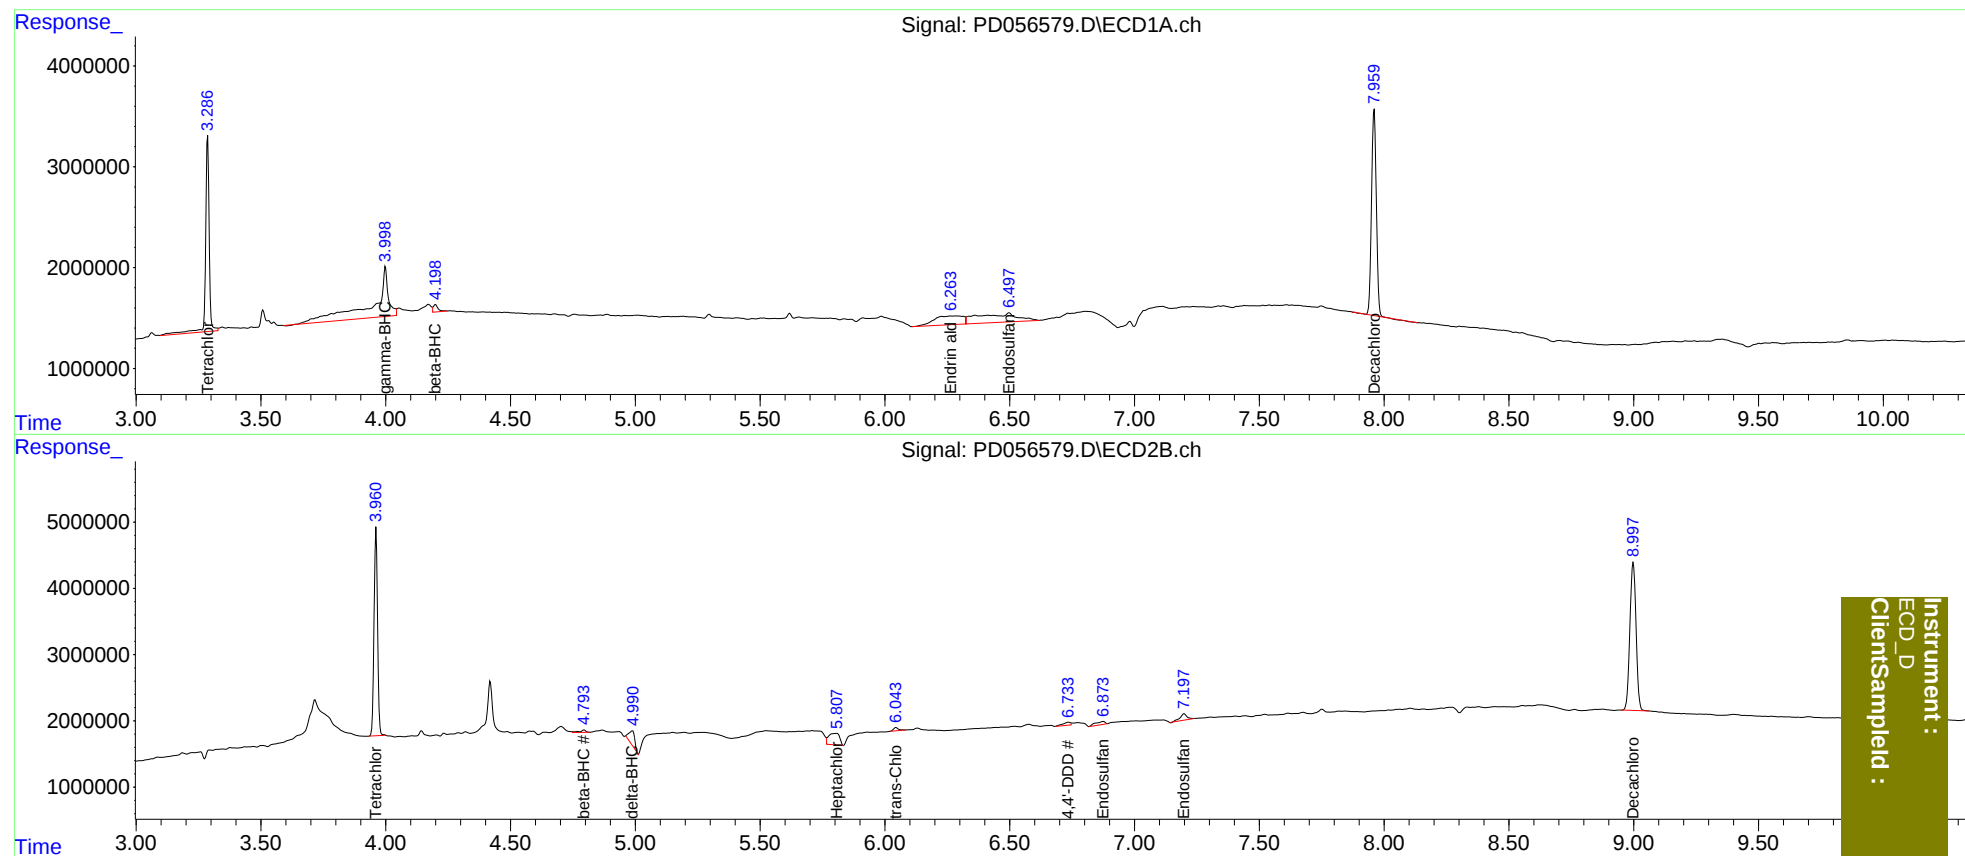

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :