

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 21:56
 Operator : SG\AJ
 Sample : K6276-22MS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:46:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.961	61919983	31029755	74.765	25.810 #
27)	SA Decachlor...	7.961	8.998	33728192	47257349	37.352	39.278
Target Compounds							
3)	MA gamma-BHC...	3.989	4.630	65242980	35845456	58.100	22.211 #
4)	MA Heptachlor	4.273	5.137	76112631	106.1E6	75.515	65.072
5)	MB Aldrin	4.513	5.440	55730418	100.3E6	51.318	61.048
6)	B beta-BHC	4.273f	0.000	76112631	0	141.410	N.D. #
7)	B delta-BHC	4.393f	5.006	21202696	22751722	18.077	13.659
12)	B 4,4'-DDE	0.000	6.287	0	875327	N.D.	0.557
13)	MA Dieldrin	5.520	6.436	110.6E6	197.3E6	108.881	125.568
14)	MA Endrin	5.774	6.653	91769916	154.2E6	109.813	121.810
15)	B Endosulfa...	0.000	6.873	0	1650096	N.D.	1.126
16)	A 4,4'-DDD	5.909	6.774	4881910	5989970	6.860	5.090 #
17)	MA 4,4'-DDT	6.143	7.073	75833738	138.0E6	107.773	116.718
18)	B Endrin al...	6.216	6.984	1093292	1338235	1.375	1.101
21)	B Endrin ke...	6.910	7.675	5337225	6646536	5.512	4.517
22)	Toxaphene-1	5.520	6.287	110.6E6	875327	12275.113	77.967 #
23)	Toxaphene-2	0.000	6.653	0	154.2E6	N.D.	11170.817
24)	Toxaphene-3	5.909	7.073	4881910	138.0E6	589.952	7014.147 #
25)	Toxaphene-4	6.143	7.073	75833738	138.0E6	3060.843	2498.903
26)	Toxaphene-5	0.000	7.627	0	2071176	N.D.	81.035

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 21:56
Operator : SG\AJ
Sample : K6276-22MS
Misc :
ALS Vial : 49 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:46:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

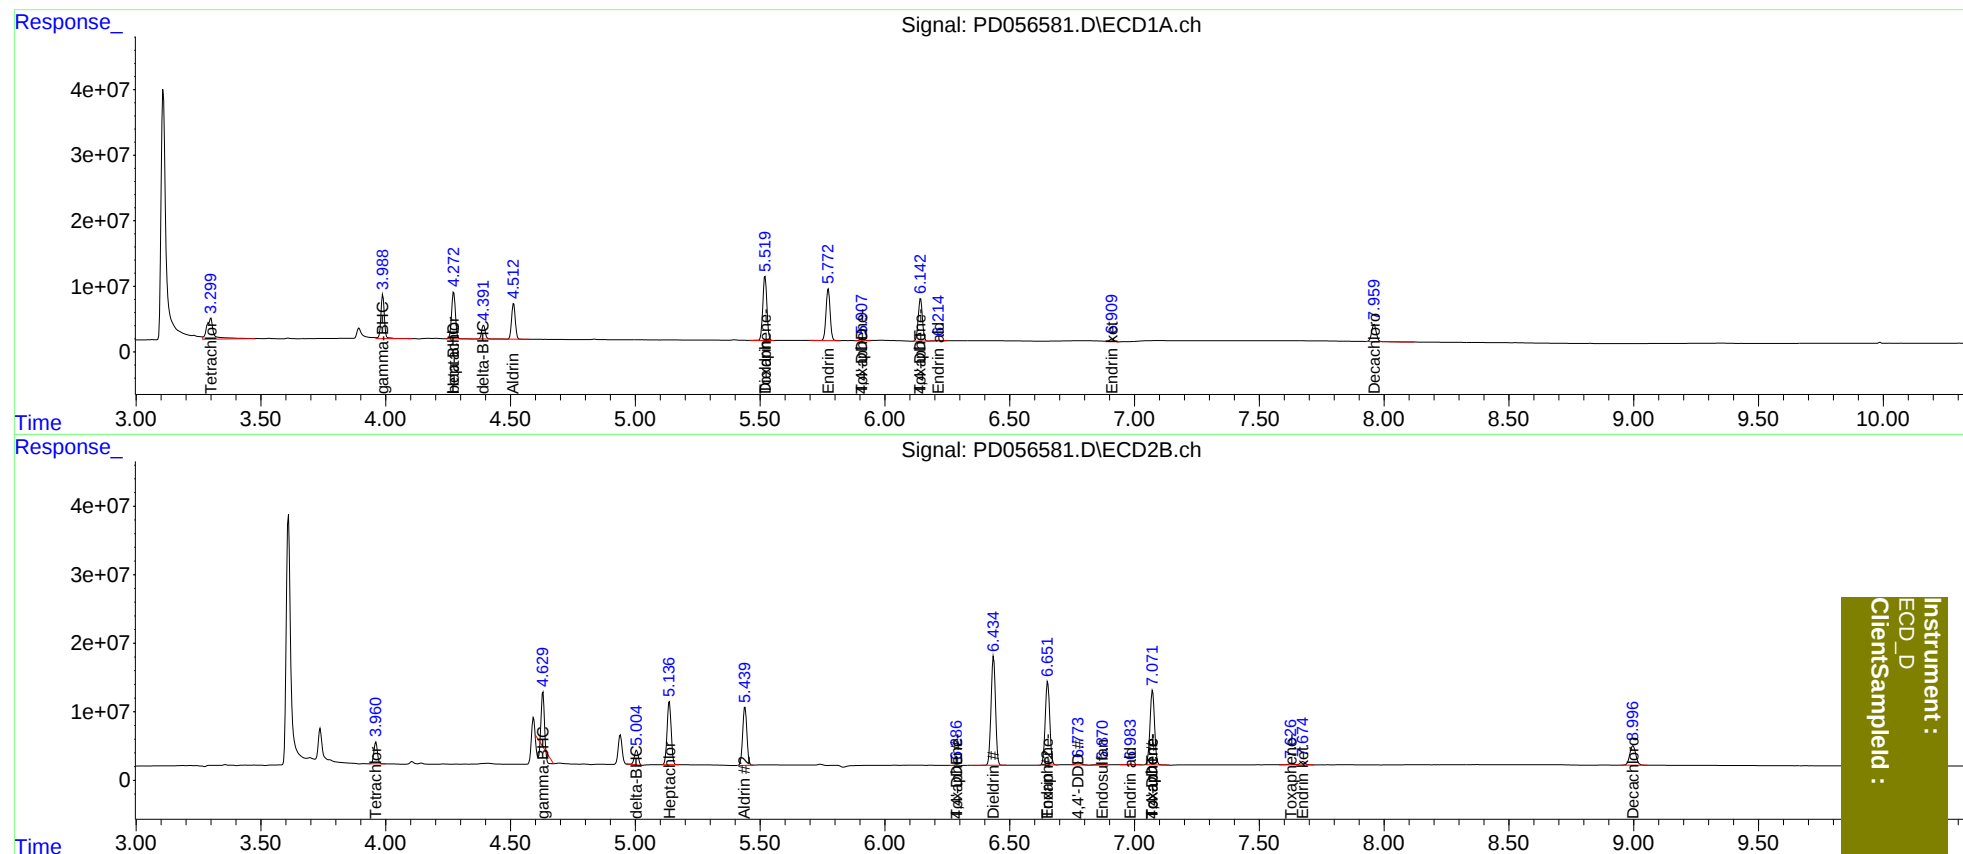

Instrument :
ECD_D
ClientSampled :
K6276-22MS

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :