

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 22:10
 Operator : SG\AJ
 Sample : K6276-23MSD
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:46:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.300	3.961	80793207	31447995	97.553	26.157 #
27)	SA Decachlor...	7.960	8.998	34629752	47838266	38.351	39.761
Target Compounds							
3)	MA gamma-BHC...	3.989	4.630	72052769	38101155	64.164	23.609 #
4)	MA Heptachlor	4.273	5.137	74613675	106.7E6	74.027	65.447
5)	MB Aldrin	4.513	5.440	56113023	100.7E6	51.670	61.298
6)	B beta-BHC	4.273f	0.000	74613675	0	138.626	N.D. #
7)	B delta-BHC	4.393f	5.005	20039335	21185586	17.086	12.719 #
12)	B 4,4'-DDE	0.000	6.286	0	981879	N.D.	0.625
13)	MA Dieldrin	5.520	6.435	111.3E6	197.4E6	109.593	125.593
14)	MA Endrin	5.773	6.652	91954247	154.0E6	110.034	121.722
15)	B Endosulfa...	0.000	6.874	0	1551383	N.D.	1.059
16)	A 4,4'-DDD	5.908	6.774	4731304	6194630	6.648	5.264
17)	MA 4,4'-DDT	6.143	7.072	76459198	137.5E6	108.662	116.296
18)	B Endrin al...	6.215	6.984	1288928	1382434	1.622	1.137 #
21)	B Endrin ke...	6.909	7.675	5668825	6811560	5.854	4.629
22)	Toxaphene-1	5.520	6.286	111.3E6	981879	12355.420	87.458 #
23)	Toxaphene-2	0.000	6.652	0	154.0E6	N.D.	11162.670
24)	Toxaphene-3	5.908	7.072	4731304	137.5E6	571.752	6988.777 #
25)	Toxaphene-4	6.143	7.072	76459198	137.5E6	3086.088	2489.864
26)	Toxaphene-5	0.000	7.628	0	2417046	N.D.	94.567

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 22:10
Operator : SG\AJ
Sample : K6276-23MSD
Misc :
ALS Vial : 50 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:46:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

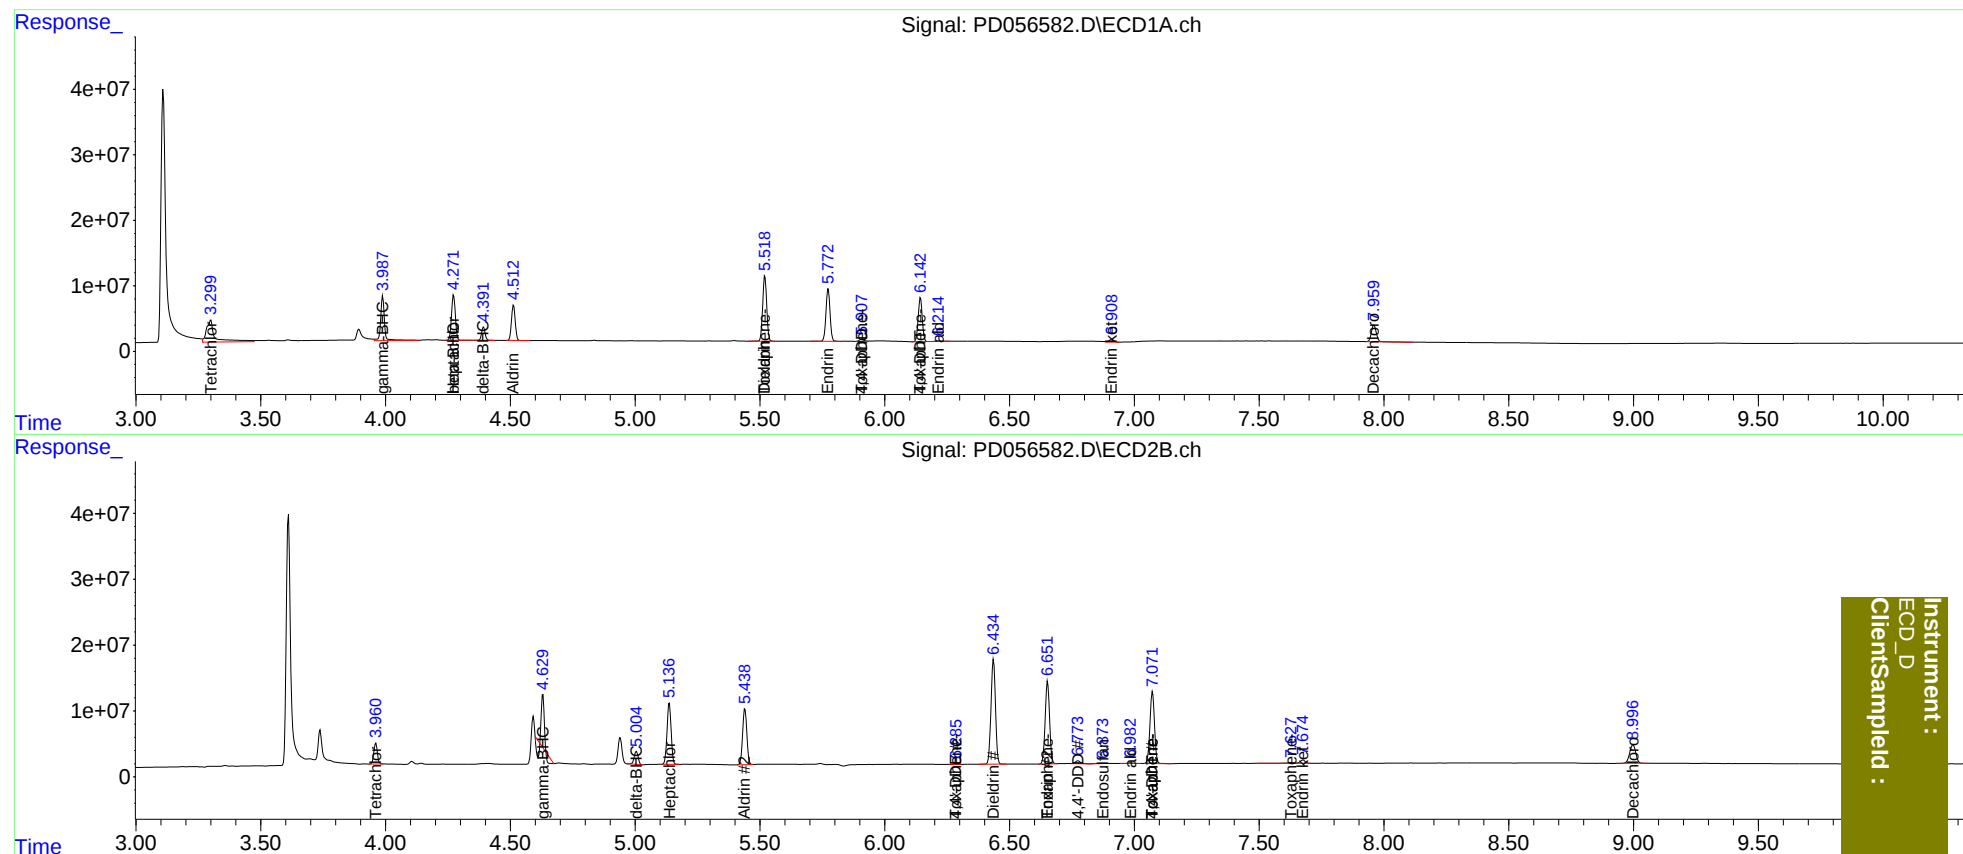

Instrument :
ECD_D
ClientSampled :

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :