

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 22:24
 Operator : SG\AJ
 Sample : K6280-12
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:46:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.961	16625387	29848042	20.074	24.827
27)	SA Decachlor...	7.960	8.997	32419135	39312150	35.903	32.674
Target Compounds							
3)	MA gamma-BHC...	3.999	4.594f	17371565	-65547	15.470	N.D. #
8)	B Heptachlo...	0.000	5.857	0	2162412	N.D.	1.396
9)	A Endosulfan I	5.275	6.130f	1789566	2064022	1.935	1.423 #
11)	B cis-Chlor...	5.275f	6.130	1789566	2064022	1.752	1.281 #
14)	MA Endrin	0.000	6.670	0	2364184	N.D.	1.868
17)	MA 4,4'-DDT	6.158	0.000	2219396	0	3.154	N.D. #
18)	B Endrin al...	6.158f	0.000	2219396	0	2.792	N.D. #
19)	B Endosulfa...	0.000	7.182	0	243440	N.D.	0.182
20)	A Methoxychlor	6.747f	0.000	1674614	0	4.941	N.D. #
23)	Toxaphene-2	0.000	6.670	0	2364184	N.D.	171.313
26)	Toxaphene-5	6.747	7.608	1674614	3280713	55.491	128.358 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 22:24
Operator : SG\AJ
Sample : K6280-12
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:46:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

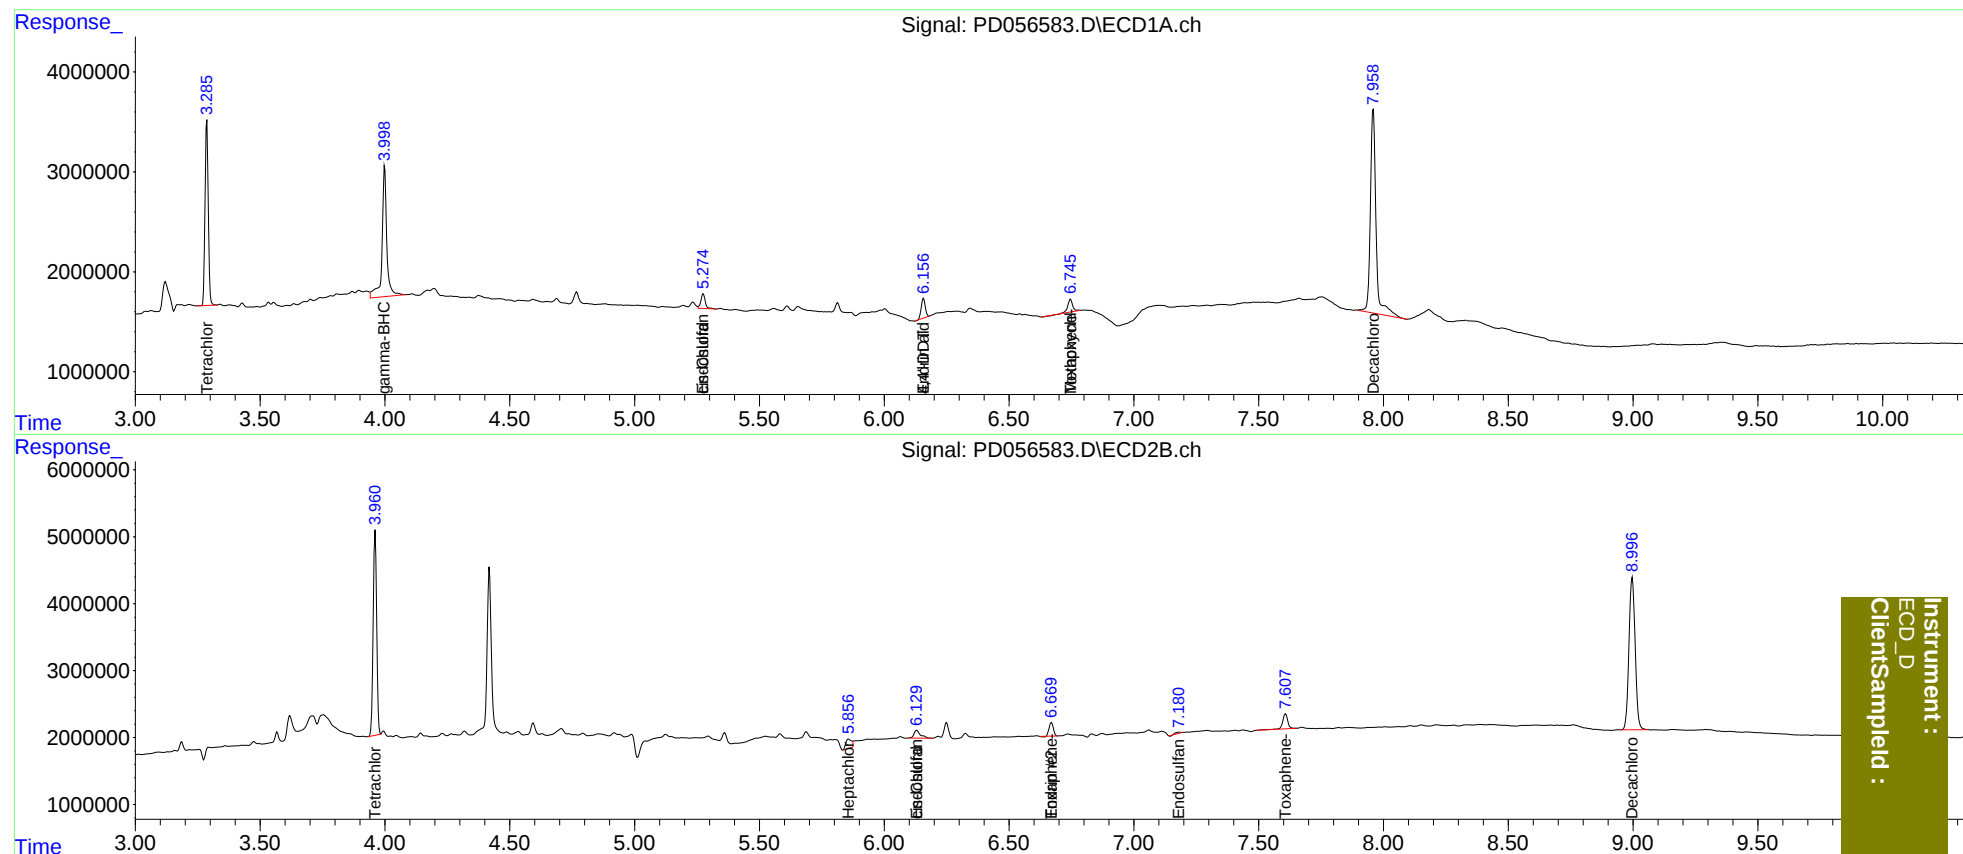

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :