

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056587.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 23:20
 Operator : SG\AJ
 Sample : K6280-10
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:47:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.961	26119082	31291587	31.537	26.027
27)	SA Decachlor...	7.960	8.998	21106000	30008584	23.374	24.942
Target Compounds							
3)	MA gamma-BHC...	3.999	4.595f	44087929	138498	39.261	<MDL #
4)	MA Heptachlor	4.290	5.125	2899923	968461	2.877	0.594 #
6)	B beta-BHC	4.290f	4.795	2899923	741993	5.388	0.900 #
7)	B delta-BHC	0.000	4.988f	0	3623184	N.D.	2.175
8)	B Heptachlo...	0.000	5.857	0	4179141	N.D.	2.698
9)	A Endosulfan I	5.235f	6.130f	1649963	5836202	1.784	4.022 #
10)	B trans-Chl...	5.235f	6.001f	1649963	451476	1.574	0.273 #
11)	B cis-Chlor...	5.235	6.130	1649963	5836202	1.616	3.621 #
12)	B 4,4'-DDE	5.421	6.328f	1038543	-289438	1.028	N.D. #
15)	B Endosulfa...	6.004f	6.829	5745018	1784583	6.031	1.218 #
16)	A 4,4'-DDD	0.000	6.829f	0	1784583	N.D.	1.517
19)	B Endosulfa...	0.000	7.180	0	408532	N.D.	0.306
21)	B Endrin ke...	0.000	7.676	0	719941	N.D.	0.489
22)	Toxaphene-1	5.421	6.328	1038543	-289438	115.268	N.D. #
23)	Toxaphene-2	5.654	0.000	3555784	0	365.407	N.D. #
24)	Toxaphene-3	6.004	0.000	5745018	0	694.254	N.D. #
26)	Toxaphene-5	0.000	7.608	0	587287	N.D.	22.978

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056587.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 23:20
Operator : SG\AJ
Sample : K6280-10
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:47:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

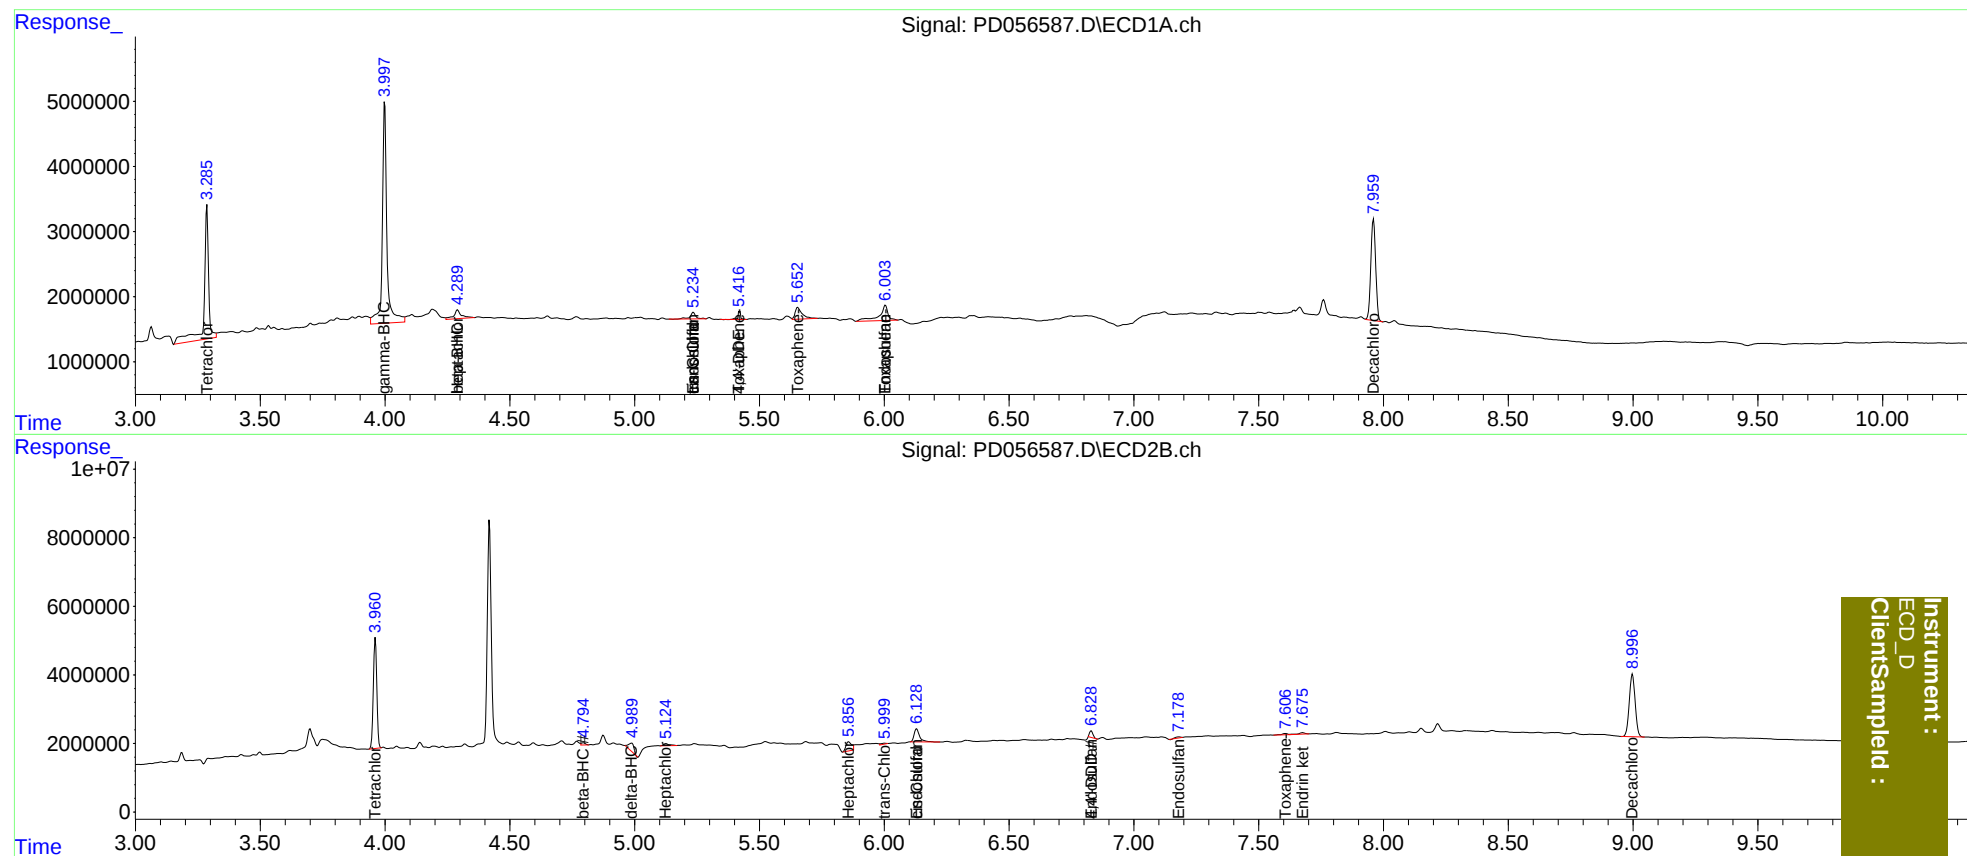

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :