

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 23:34
 Operator : SG\AJ
 Sample : K6280-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:47:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.961	17561921	28989202	21.205	24.112
27)	SA Decachlor...	7.960	8.998	25916245	35575717	28.701	29.569
Target Compounds							
3)	MA gamma-BHC...	3.998	4.659f	6291336	941848	5.603	0.584 #
4)	MA Heptachlor	4.318f	5.118	1672204	2671584	1.659	1.639
5)	MB Aldrin	4.528	5.448	12806972	1760842	11.793	1.072 #
6)	B beta-BHC	4.200f	0.000	36863770	0	68.490	N.D. #
7)	B delta-BHC	0.000	4.992	0	28455679	N.D.	17.084
8)	B Heptachlo...	0.000	5.860	0	1230605	N.D.	0.794
9)	A Endosulfan I	5.240f	6.175	1820875	6493432	1.969	4.475 #
10)	B trans-Chl...	5.240f	6.041	1820875	2591803	1.737	1.568
11)	B cis-Chlor...	5.240	6.175f	1820875	6493432	1.783	4.029 #
12)	B 4,4'-DDE	5.360f	0.000	3689043	0	3.652	N.D. #
15)	B Endosulfa...	0.000	6.873	0	1478395	N.D.	1.009
16)	A 4,4'-DDD	0.000	6.736f	0	960055	N.D.	0.816

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 23:34
Operator : SG\AJ
Sample : K6280-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:47:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

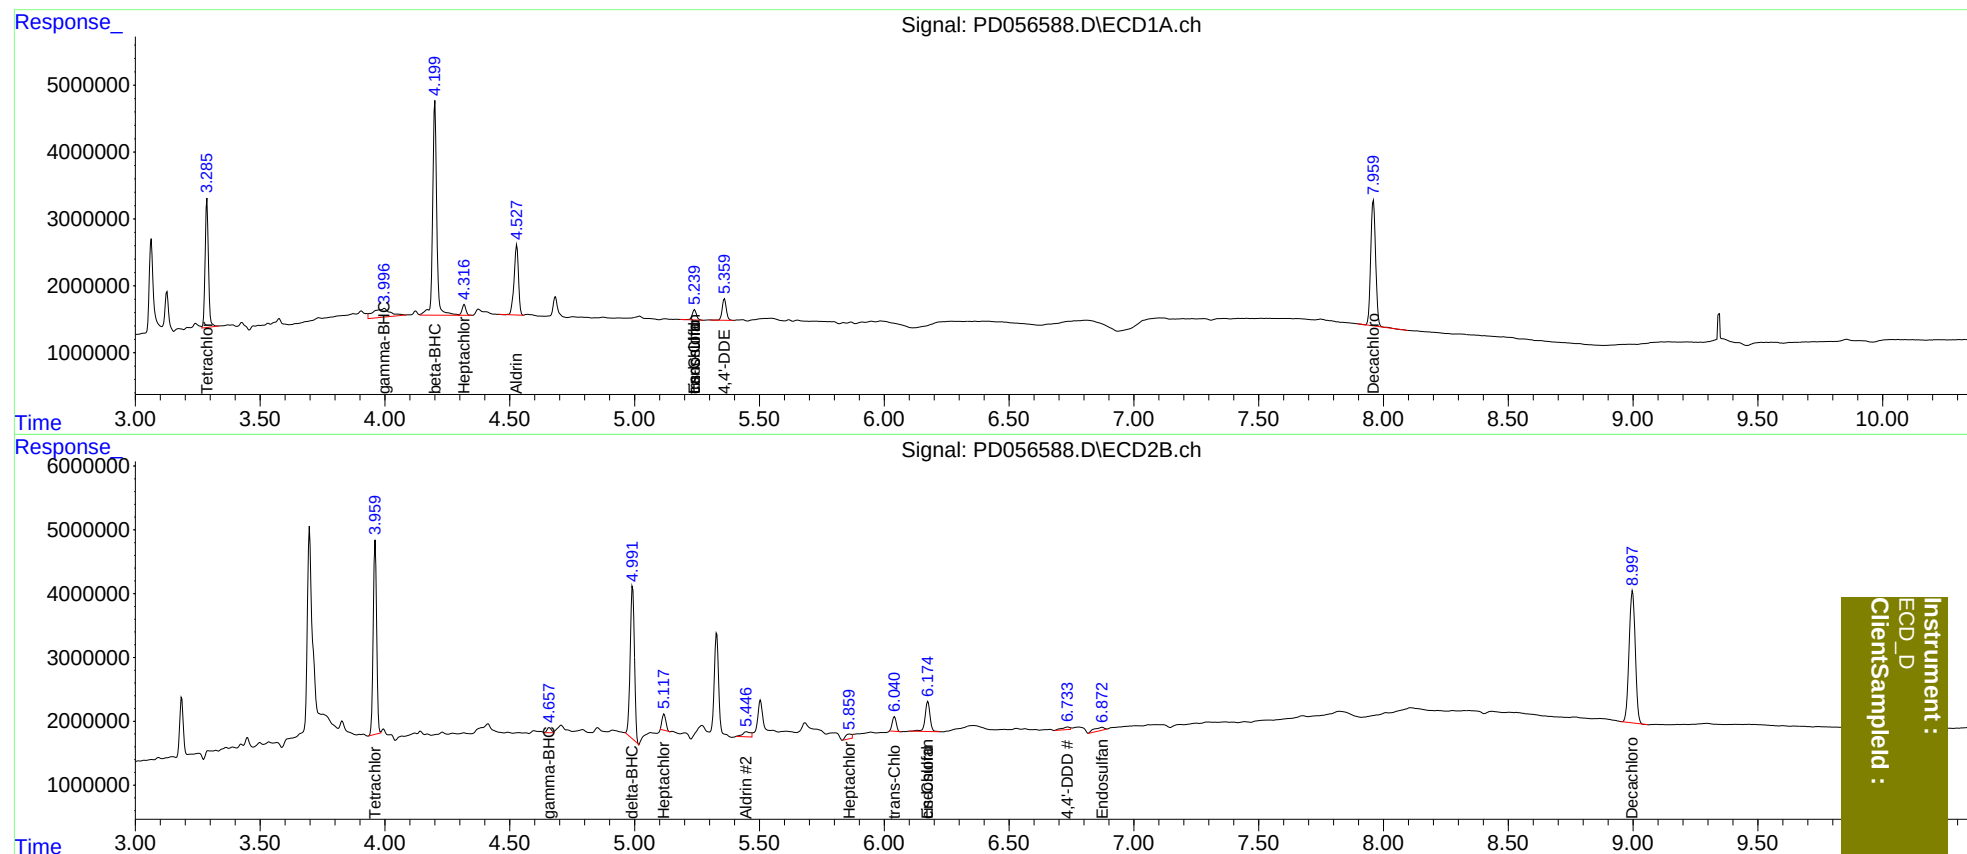

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :