

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056589.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 23:48
 Operator : SG\AJ
 Sample : K6280-11
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:47:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.961	18420070	31734193	22.241	26.396
27)	SA Decachlor...	7.960	8.997	30448223	43158139	33.720	35.871
Target Compounds							
2)	A alpha-BHC	3.701	0.000	1351436	0	1.148	N.D. #
3)	MA gamma-BHC...	4.000	0.000	12488245	0	11.121	N.D. #
6)	B beta-BHC	4.204f	0.000	3087303	0	5.736	N.D. #
8)	B Heptachlo...	0.000	5.858	0	1875555	N.D.	1.211
18)	B Endrin al...	6.257f	0.000	2814743	0	3.541	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056589.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 23:48
Operator : SG\AJ
Sample : K6280-11
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:47:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

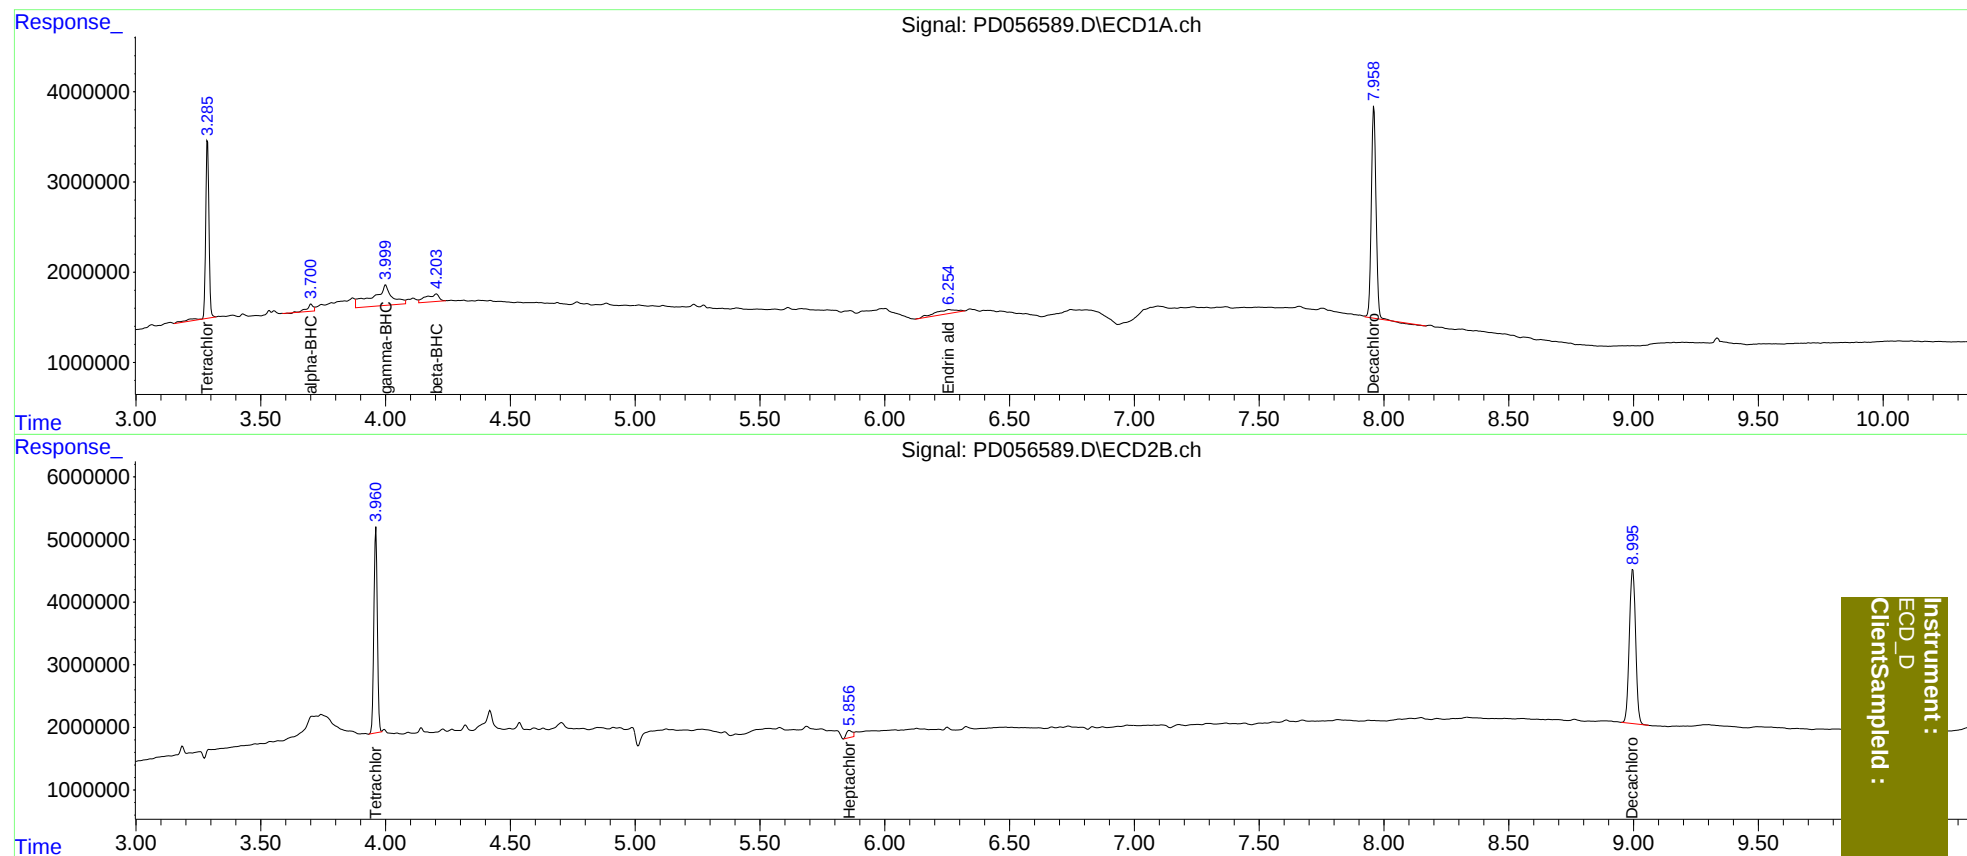

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :