

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
 Data File : PD056598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 01:55
 Operator : SG\AJ
 Sample : K6280-15
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFF37

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 04:53:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.961	16181958	28621991	19.539	23.807
27)	SA Decachlor...	7.960	8.997	20618377	30381539	22.834	25.252
Target Compounds							
5)	MB Aldrin	0.000	5.492f	0	3485068	N.D.	2.121
6)	B beta-BHC	0.000	4.769f	0	2182394	N.D.	2.648
7)	B delta-BHC	0.000	4.989f	0	3001928	N.D.	1.802
8)	B Heptachlo...	0.000	5.856	0	3371113	N.D.	2.176
10)	B trans-Chl...	0.000	6.002f	0	608812	N.D.	0.368
15)	B Endosulfa...	0.000	6.828f	0	1157501	N.D.	0.790
16)	A 4,4'-DDD	0.000	6.828f	0	1157501	N.D.	0.984
19)	B Endosulfa...	0.000	7.257f	0	627370	N.D.	0.469


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121819\
Data File : PD056598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 01:55
Operator : SG\AJ
Sample : K6280-15
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFF37

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 04:53:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

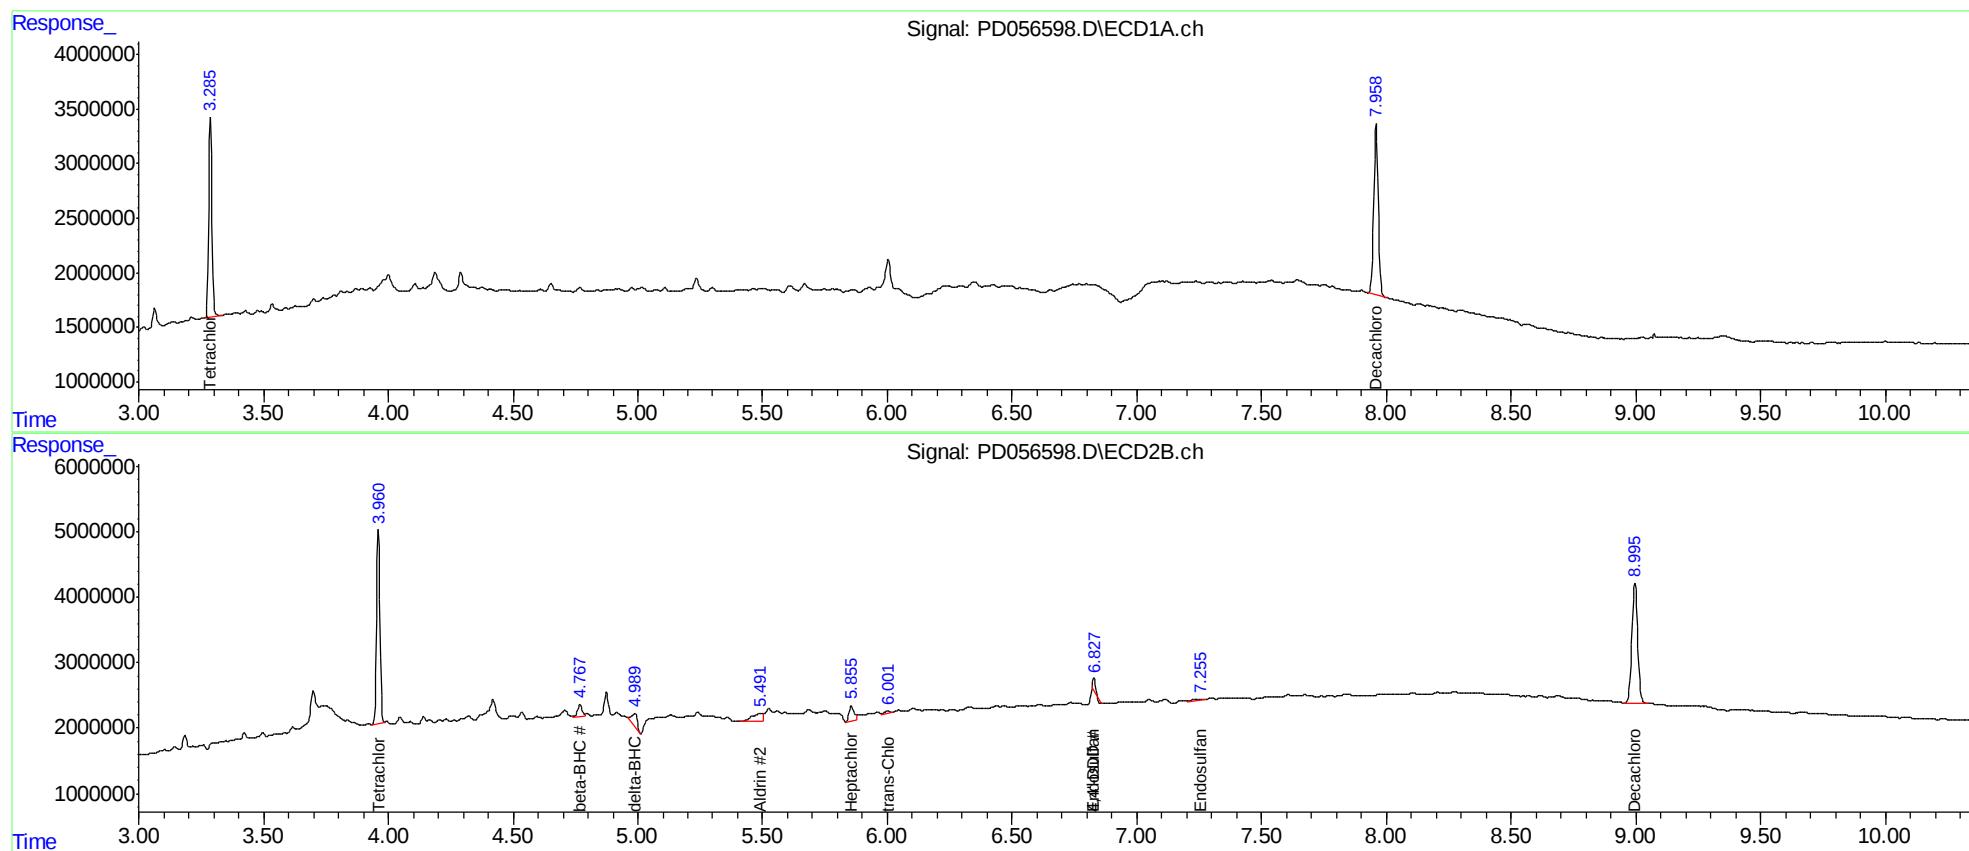


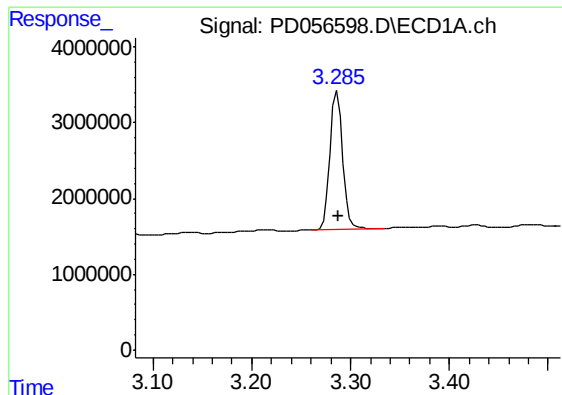

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: -0.001 min
Response: 16181958
Conc: 19.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFF37

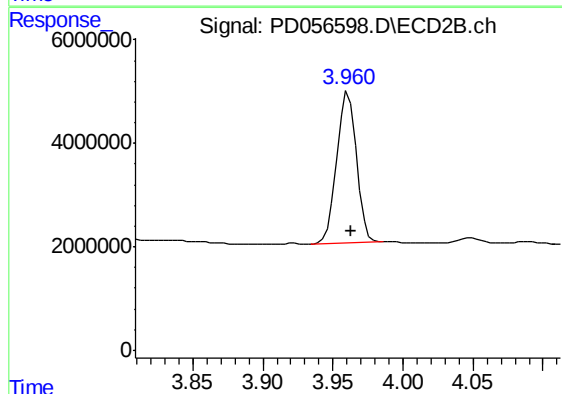


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.002 min
Response: 28621991
Conc: 23.81 ng/ml

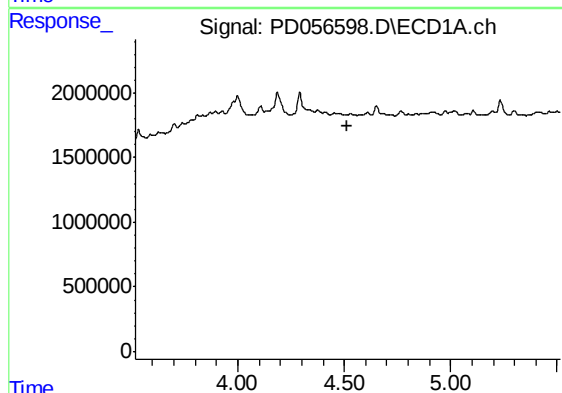


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.516 min
Response: 0
Conc: N.D.

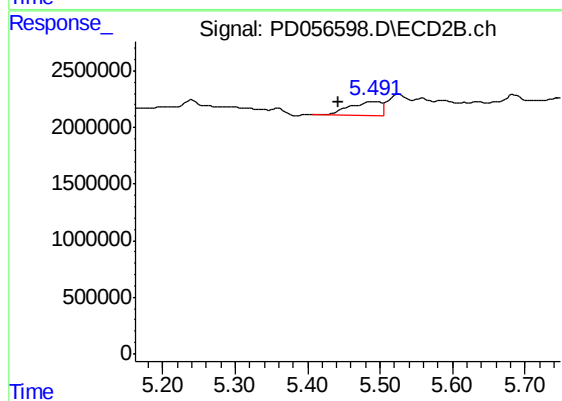

#5 Aldrin


R.T.: 5.492 min
Delta R.T.: 0.050 min
Response: 3485068
Conc: 2.12 ng/ml

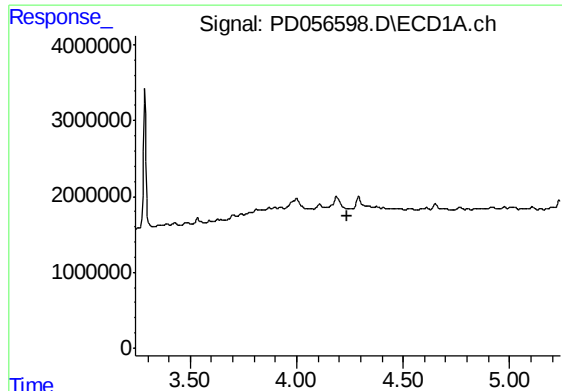

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFF37

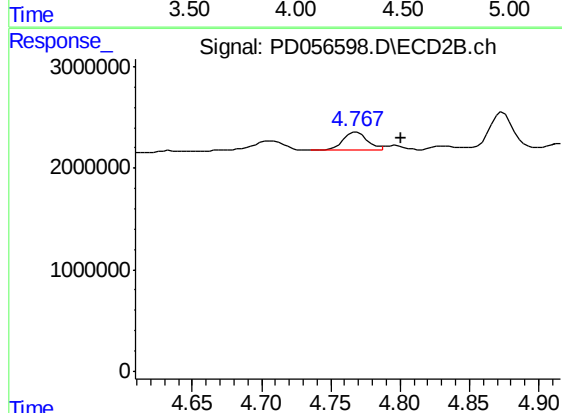


#6 beta-BHC

R.T.: 4.769 min
Delta R.T.: -0.032 min
Response: 2182394
Conc: 2.65 ng/ml

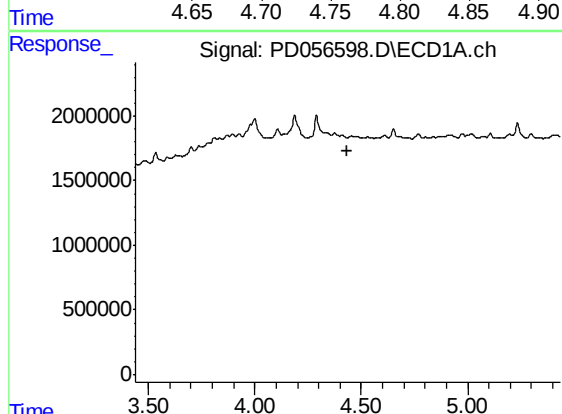


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

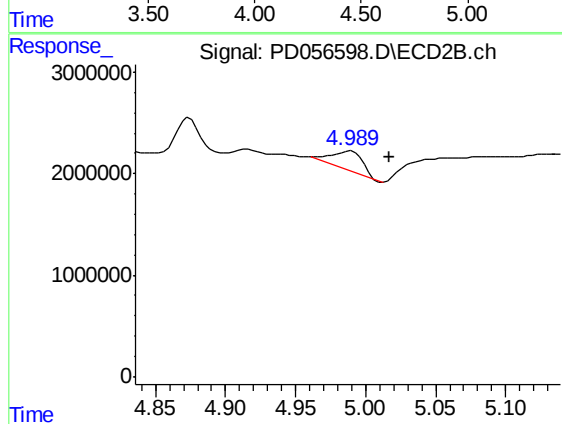

#7 delta-BHC


R.T.: 4.989 min
Delta R.T.: -0.028 min
Response: 3001928
Conc: 1.80 ng/ml

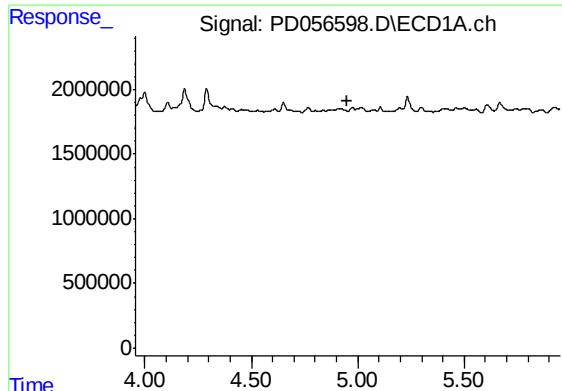

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFF37

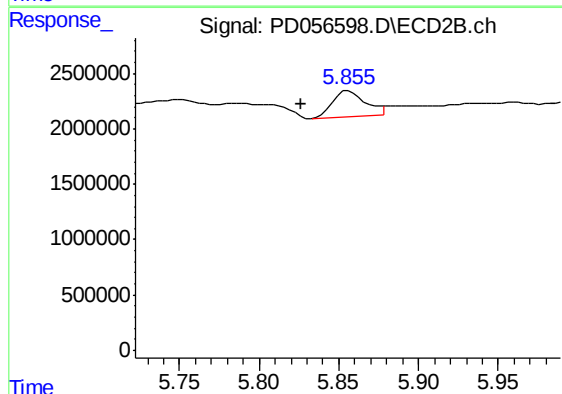


#8 Heptachlor epoxide

R.T.: 5.856 min
Delta R.T.: 0.030 min
Response: 3371113
Conc: 2.18 ng/ml

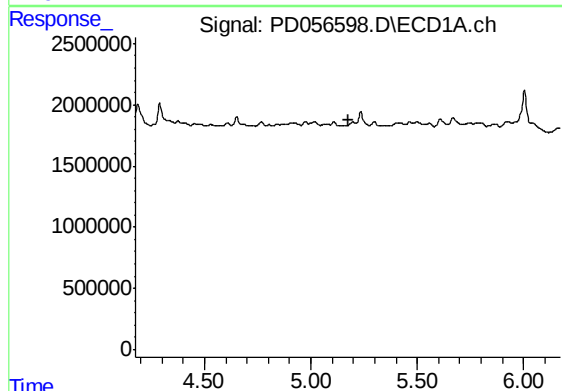


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

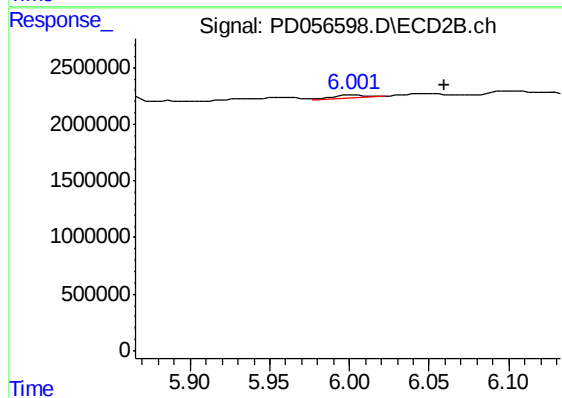

#10 trans-Chlordane


R.T.: 6.002 min
Delta R.T.: -0.058 min
Response: 608812
Conc: 0.37 ng/ml

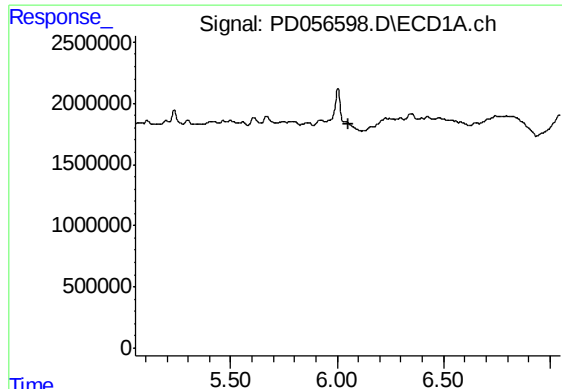

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFF37

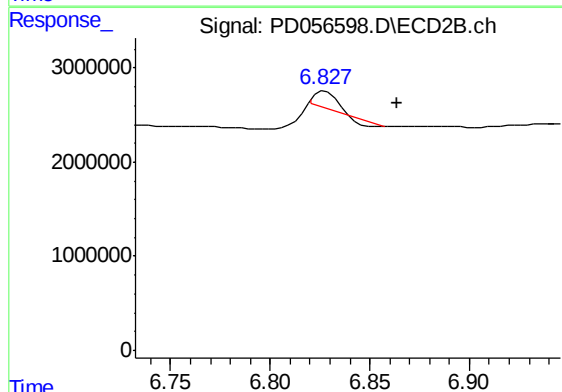


#15 Endosulfan II

R.T.: 6.828 min
Delta R.T.: -0.036 min
Response: 1157501
Conc: 0.79 ng/ml

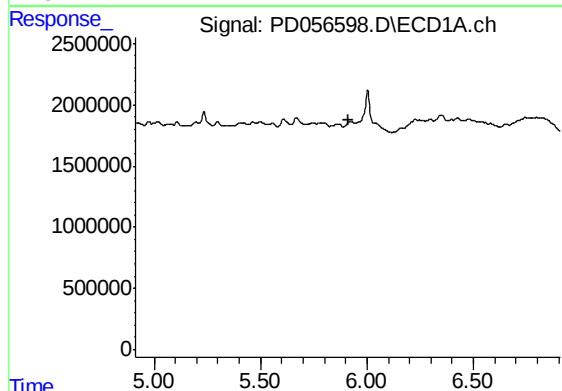


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

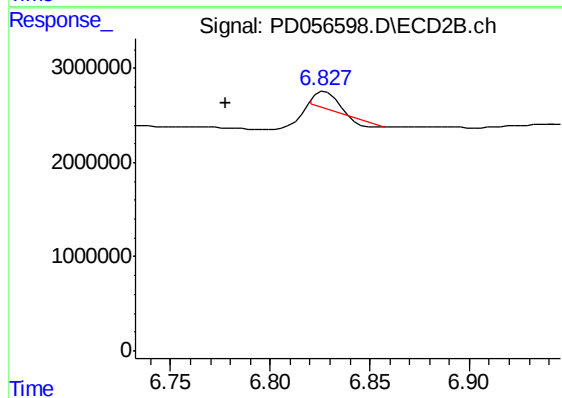

#16 4,4'-DDD


R.T.: 6.828 min
Delta R.T.: 0.050 min
Response: 1157501
Conc: 0.98 ng/ml

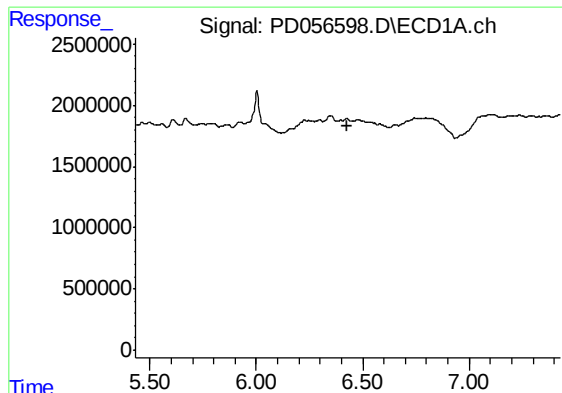

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFF37

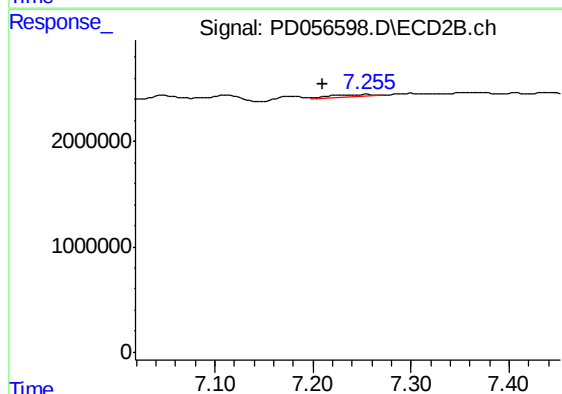


#19 Endosulfan Sulfate

R.T.: 7.257 min
Delta R.T.: 0.047 min
Response: 627370
Conc: 0.47 ng/ml

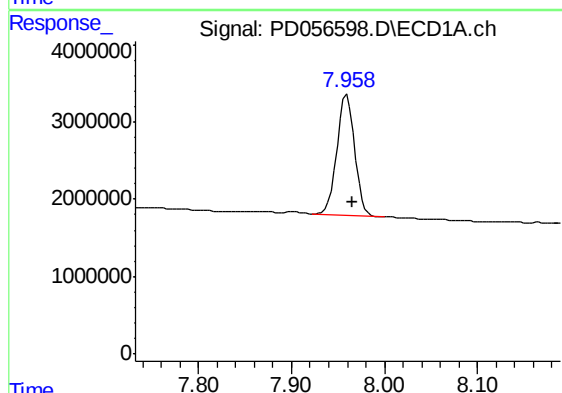

#27 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.006 min
Response: 20618377
Conc: 22.83 ng/ml

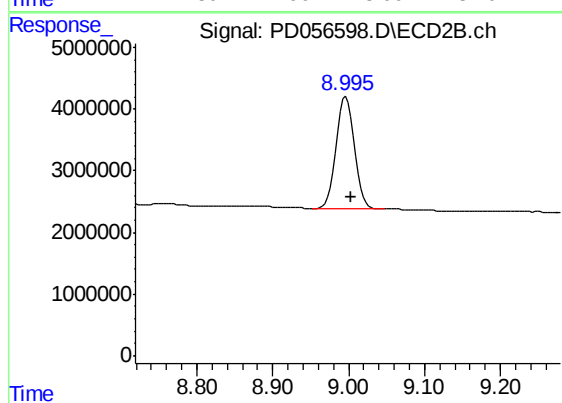

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: -0.006 min
Response: 30381539
Conc: 25.25 ng/ml