

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121824\
 Data File : PD087159.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2024 16:23
 Operator : AR\AJ
 Sample : P5226-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2AP5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/19/2024
 Supervised By : Ankita Jodhani 12/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:27:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.555	2.883	30856894	174.8E6	16.780	15.145
27) SA Decachlor...	9.090	8.085	65965801	177.1E6	24.776m	13.895 #
Target Compounds						
9) A Endosulfan I	6.101	5.274	5498656	118.4E6	1.849m	8.181m#
13) MA Dieldrin	6.354	5.518	2608561	25158169	0.796m	1.647m#
14) MA Endrin	6.581	5.786	1715142	16787794	0.635m	1.215m#
19) B Endosulfa...	7.156	6.505	1240374	10686658	0.460m	0.796m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121824\
Data File : PD087159.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2024 16:23
Operator : AR\AJ
Sample : P5226-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:27:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

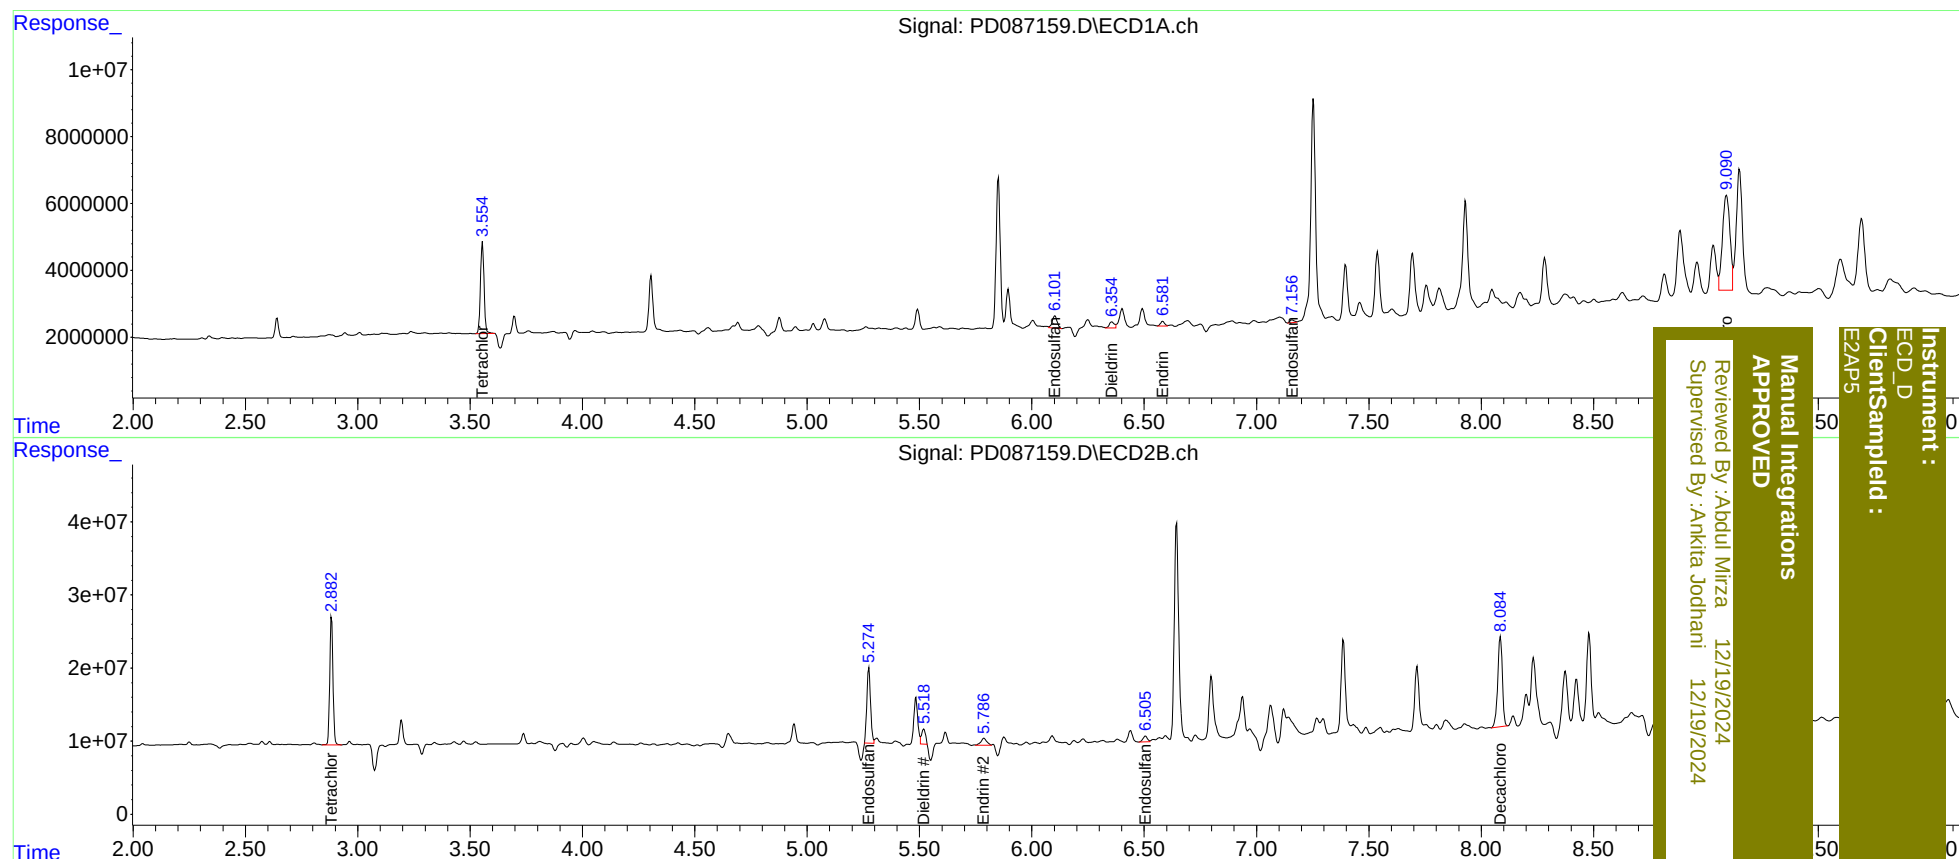

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 12/19/2024
Supervised By: Ankita Jodhani 12/19/2024

Instrument :
ECD_D
ClientSampled :
EZAP5