

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121824\
 Data File : PD087175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2024 21:02
 Operator : AR\AJ
 Sample : P5226-25MS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2AR4MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/19/2024
 Supervised By :Ankita Jodhani 12/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:33:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.883	25624042	155.6E6	13.934m	13.479
27)	SA Decachlor...	9.084	8.085	29878706	141.1E6	11.222	11.067
Target Compounds							
2)	A alpha-BHC	4.003	3.397	156.5E6	669.9E6	44.441m	37.400
3)	MA gamma-BHC...	4.336	3.734	153.2E6	627.3E6	43.987	37.608
4)	MA Heptachlor	4.936	4.089	151.7E6	632.5E6	43.658	36.772
5)	MB Aldrin	5.279	4.375	146.6E6	616.8E6	41.504	36.108
6)	B beta-BHC	4.520	4.030	62061642	276.1E6	39.151	34.955
7)	B delta-BHC	4.768	4.267	105.7E6	438.2E6	29.034	24.958
8)	B Heptachlo...	5.698	4.880	133.2E6	562.8E6	40.763	35.487
9)	A Endosulfan I	6.081	5.255	123.6E6	531.0E6	41.566	36.685
10)	B trans-Chl...	5.952	5.132	126.8E6	587.8E6	39.635	35.589m
11)	B cis-Chlor...	6.035	5.198	133.9E6	577.3E6	41.152	36.023
12)	B 4,4'-DDE	6.203	5.384	252.5E6	1092.7E6	81.872	71.667
13)	MA Dieldrin	6.354	5.521	275.4E6	1115.4E6	84.014	73.003
14)	MA Endrin	6.582	5.798	230.4E6	1025.9E6	85.219	74.260
15)	B Endosulfa...	6.793	6.089	216.0E6	965.4E6	77.830	69.186
16)	A 4,4'-DDD	6.712	5.938	195.7E6	878.9E6	82.509	72.750
17)	MA 4,4'-DDT	7.027	6.193	206.0E6	941.9E6	83.105m	72.854
18)	B Endrin al...	6.921	6.268	163.3E6	709.9E6	74.306	66.148
19)	B Endosulfa...	7.156	6.491	198.3E6	893.3E6	73.520	66.568
20)	A Methoxychlor	7.500	6.765	532.0E6	2014.9E6	394.155	348.505
21)	B Endrin ke...	7.637	7.000	233.2E6	1021.2E6	76.460	68.342

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121824\
Data File : PD087175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2024 21:02
Operator : AR\AJ
Sample : P5226-25MS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:33:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

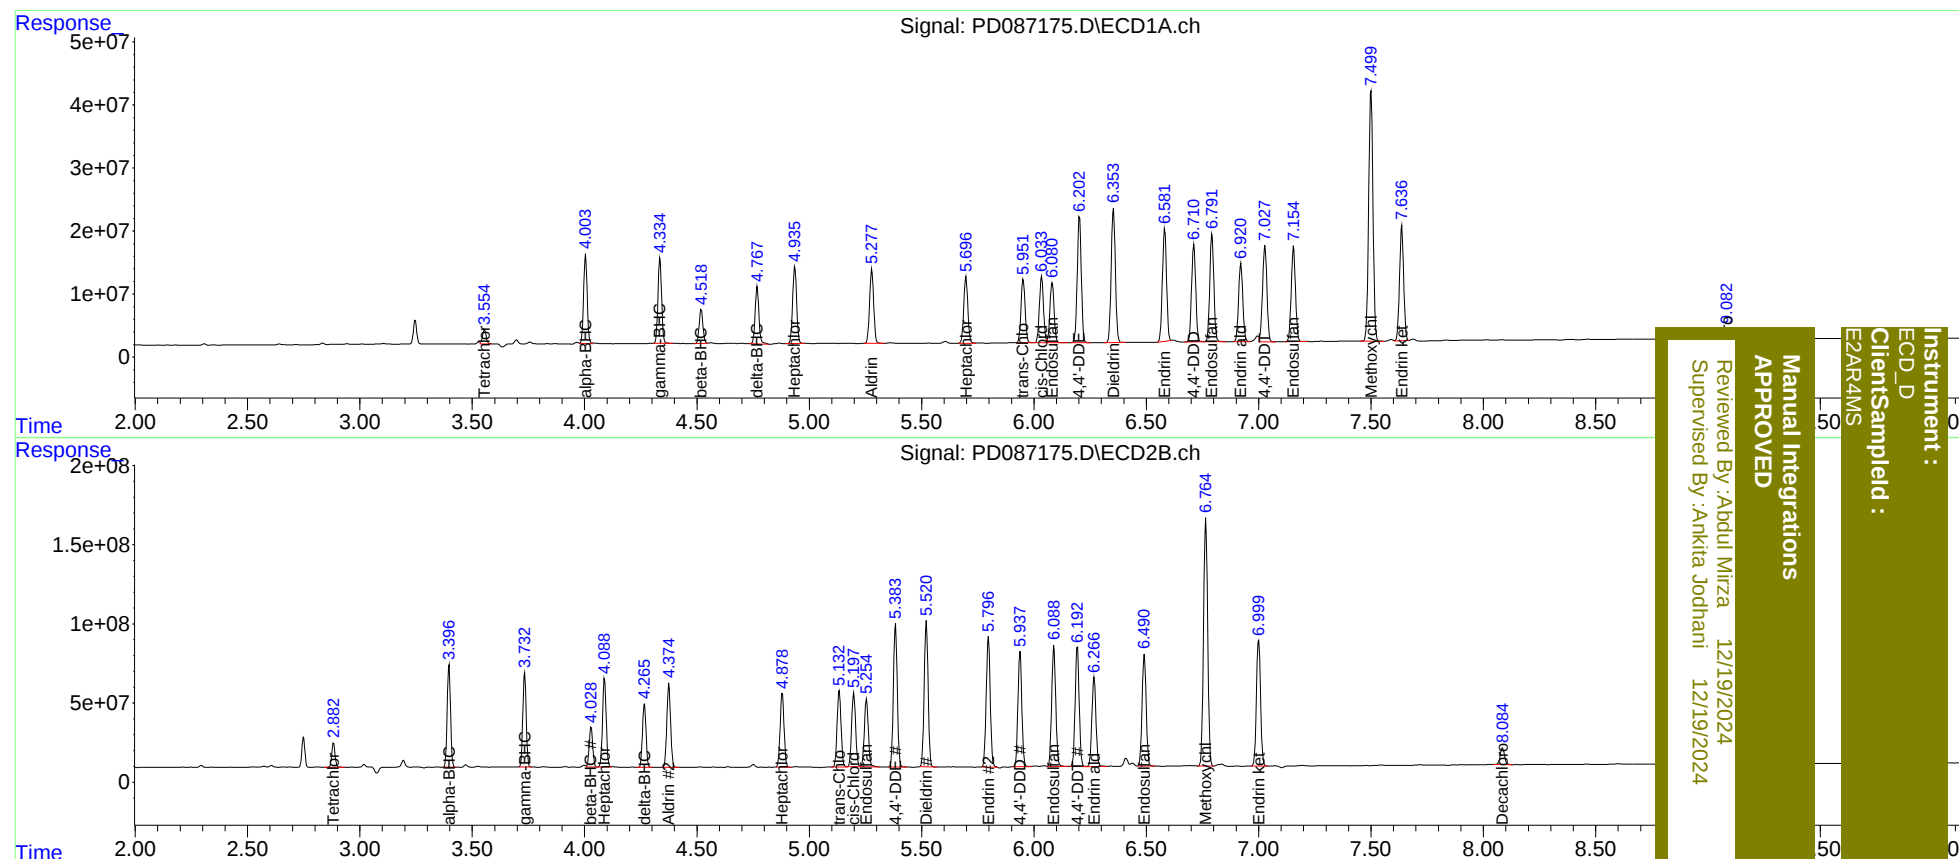

Instrument :
ECD_D
ClientSampled :
EZAR4MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 12/19/2024
Supervised By: Ankita Jodhani 12/19/2024