

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121824\
 Data File : PD087176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2024 21:16
 Operator : AR\AJ
 Sample : P5226-26MSD
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2AR4MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/19/2024
 Supervised By :Ankita Jodhani 12/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:34:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.883	25679745	154.2E6	13.965m	13.360
27)	SA Decachlor...	9.085	8.086	29986168	140.8E6	11.262	11.044
Target Compounds							
2)	A alpha-BHC	4.004	3.397	157.5E6	666.5E6	44.743m	37.210
3)	MA gamma-BHC...	4.336	3.734	154.0E6	626.1E6	44.230	37.540
4)	MA Heptachlor	4.936	4.090	152.0E6	629.9E6	43.753	36.619
5)	MB Aldrin	5.279	4.376	147.3E6	615.5E6	41.708	36.033
6)	B beta-BHC	4.520	4.030	62345277	274.3E6	39.330	34.729
7)	B delta-BHC	4.768	4.267	105.5E6	436.4E6	28.980	24.851
8)	B Heptachlo...	5.698	4.880	133.3E6	563.1E6	40.780	35.508
9)	A Endosulfan I	6.082	5.256	123.8E6	532.2E6	41.630	36.774
10)	B trans-Chl...	5.953	5.133	128.2E6	590.5E6	40.073	35.751m
11)	B cis-Chlor...	6.034	5.199	134.4E6	577.4E6	41.306	36.034
12)	B 4,4'-DDE	6.203	5.385	253.6E6	1095.2E6	82.234	71.828
13)	MA Dieldrin	6.355	5.521	276.7E6	1117.9E6	84.421	73.166
14)	MA Endrin	6.582	5.798	233.0E6	1024.0E6	86.209	74.122
15)	B Endosulfa...	6.793	6.090	221.1E6	965.3E6	79.671	69.179
16)	A 4,4'-DDD	6.712	5.939	196.6E6	882.4E6	82.877	73.040
17)	MA 4,4'-DDT	7.027	6.194	208.2E6	939.7E6	84.000m	72.685
18)	B Endrin al...	6.922	6.268	161.2E6	695.9E6	73.332	64.841
19)	B Endosulfa...	7.156	6.492	199.1E6	891.5E6	73.811	66.434
20)	A Methoxychlor	7.500	6.766	533.0E6	2016.8E6	394.877	348.834
21)	B Endrin ke...	7.637	7.001	233.5E6	1020.4E6	76.551	68.287

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121824\
Data File : PD087176.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2024 21:16
Operator : AR\AJ
Sample : P5226-26MSD
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:34:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

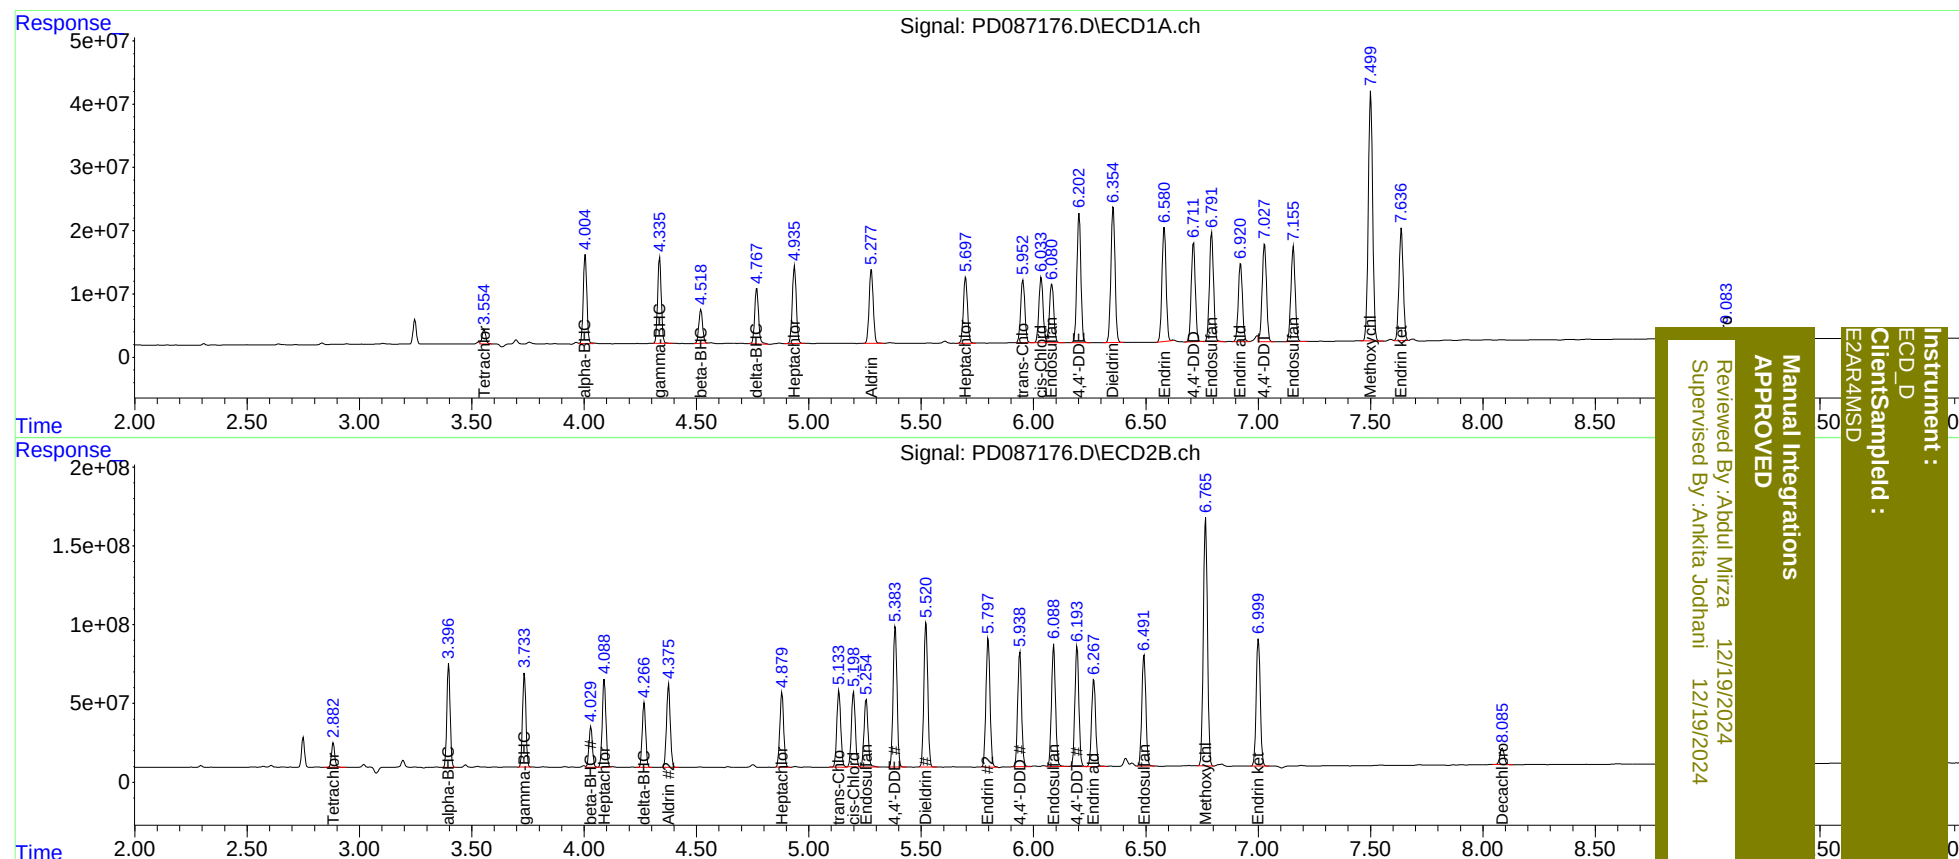

Instrument :
ECD_D
Client Sampled :
EZAR4MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 12/19/2024
Supervised By: Ankita Jodhani 12/19/2024