

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121824\
 Data File : PD087152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2024 14:13
 Operator : AR\AJ
 Sample : PB165686BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS686

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/19/2024
 Supervised By :Ankita Jodhani 12/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:24:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	38301788	228.5E6	20.828	19.795
27)	SA Decachlor...	9.084	8.085	58868197	274.6E6	22.110	21.546
Target Compounds							
2)	A alpha-BHC	4.004	3.396	13904688	79678773	3.949	4.449
3)	MA gamma-BHC...	4.334	3.734	14669093	76439291	4.212m	4.583
4)	MA Heptachlor	4.936	4.089	15336431	78050866	4.414	4.537
5)	MB Aldrin	5.278	4.375	14581758	78272988	4.130	4.582
6)	B beta-BHC	4.520	4.029	6638217	35281528	4.188	4.466
7)	B delta-BHC	4.769	4.266	16124296	74222300	4.431	4.227
8)	B Heptachlo...	5.697	4.879	13918494	74669455	4.258m	4.708
9)	A Endosulfan I	6.080	5.254	13257259	68664829	4.459m	4.744
10)	B trans-Chl...	5.953	5.132	12696661	74954056	3.970	4.538m
11)	B cis-Chlor...	6.033	5.198	14496957	74373710	4.456m	4.641
12)	B 4,4'-DDE	6.203	5.383	24517125	137.7E6	7.949	9.033
13)	MA Dieldrin	6.354	5.520	27561192	140.7E6	8.408	9.211
14)	MA Endrin	6.581	5.795	22793009	129.7E6	8.432	9.391m
15)	B Endosulfa...	6.793	6.088	22379219	127.9E6	8.065	9.164
16)	A 4,4'-DDD	6.711	5.938	19618109	117.9E6	8.269	9.758
17)	MA 4,4'-DDT	7.027	6.193	20528733	113.1E6	8.282m	8.751
18)	B Endrin al...	6.921	6.267	19788469	103.5E6	9.003	9.647
19)	B Endosulfa...	7.156	6.491	23151035	125.7E6	8.581	9.367
20)	A Methoxychlor	7.501	6.764	60587592	276.6E6	44.889	47.844
21)	B Endrin ke...	7.637	7.000	25134797	135.5E6	8.240	9.069

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121824\
Data File : PD087152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2024 14:13
Operator : AR\AJ
Sample : PB165686BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:24:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

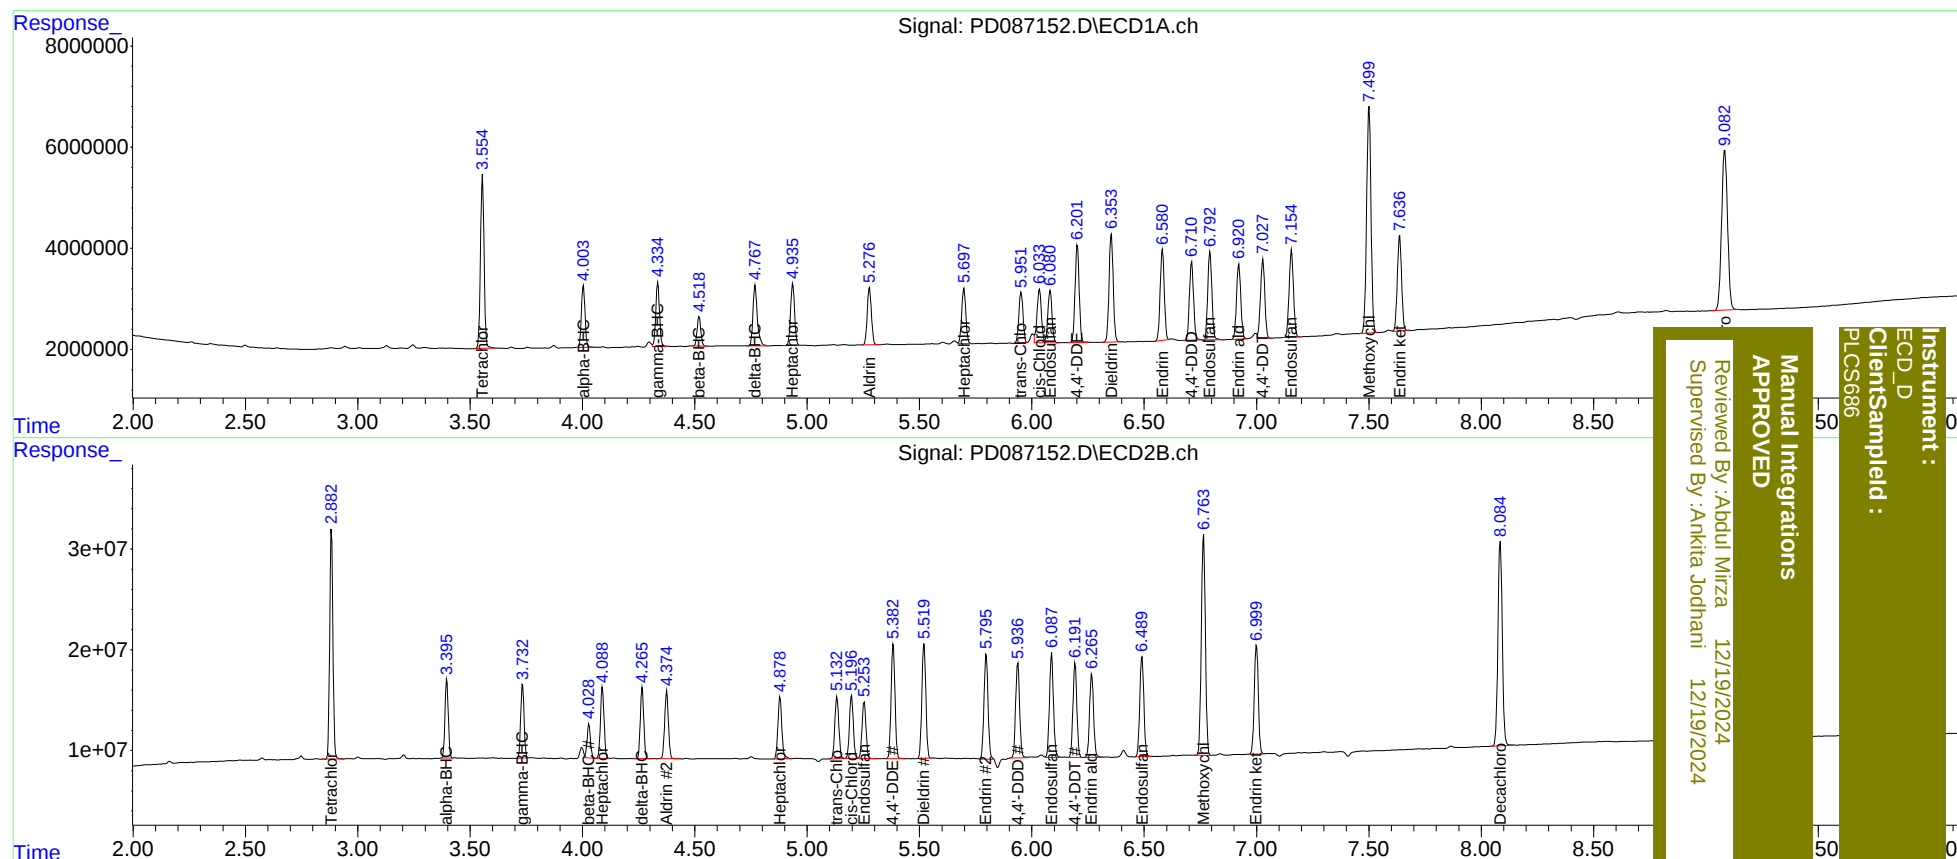

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 12/19/2024
Supervised By: Ankita Jodhani 12/19/2024

Instrument :
ECD_D
Client Sampled :
PLCS686