

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
 Data File : PD056616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 13:22
 Operator : SG\AJ
 Sample : K6308-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0C75

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 00:40:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.286	3.961	15485937	27955975	18.698	23.253
27) SA Decachlor...	7.958	8.995	26128104	38052245	28.936	31.627
Target Compounds						
6) B beta-BHC	0.000	4.841f	0	1338378	N.D.	1.624
8) B Heptachlo...	0.000	5.800	0	7898632	N.D.	5.098


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
Data File : PD056616.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 13:22
Operator : SG\AJ
Sample : K6308-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0C75

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 00:40:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

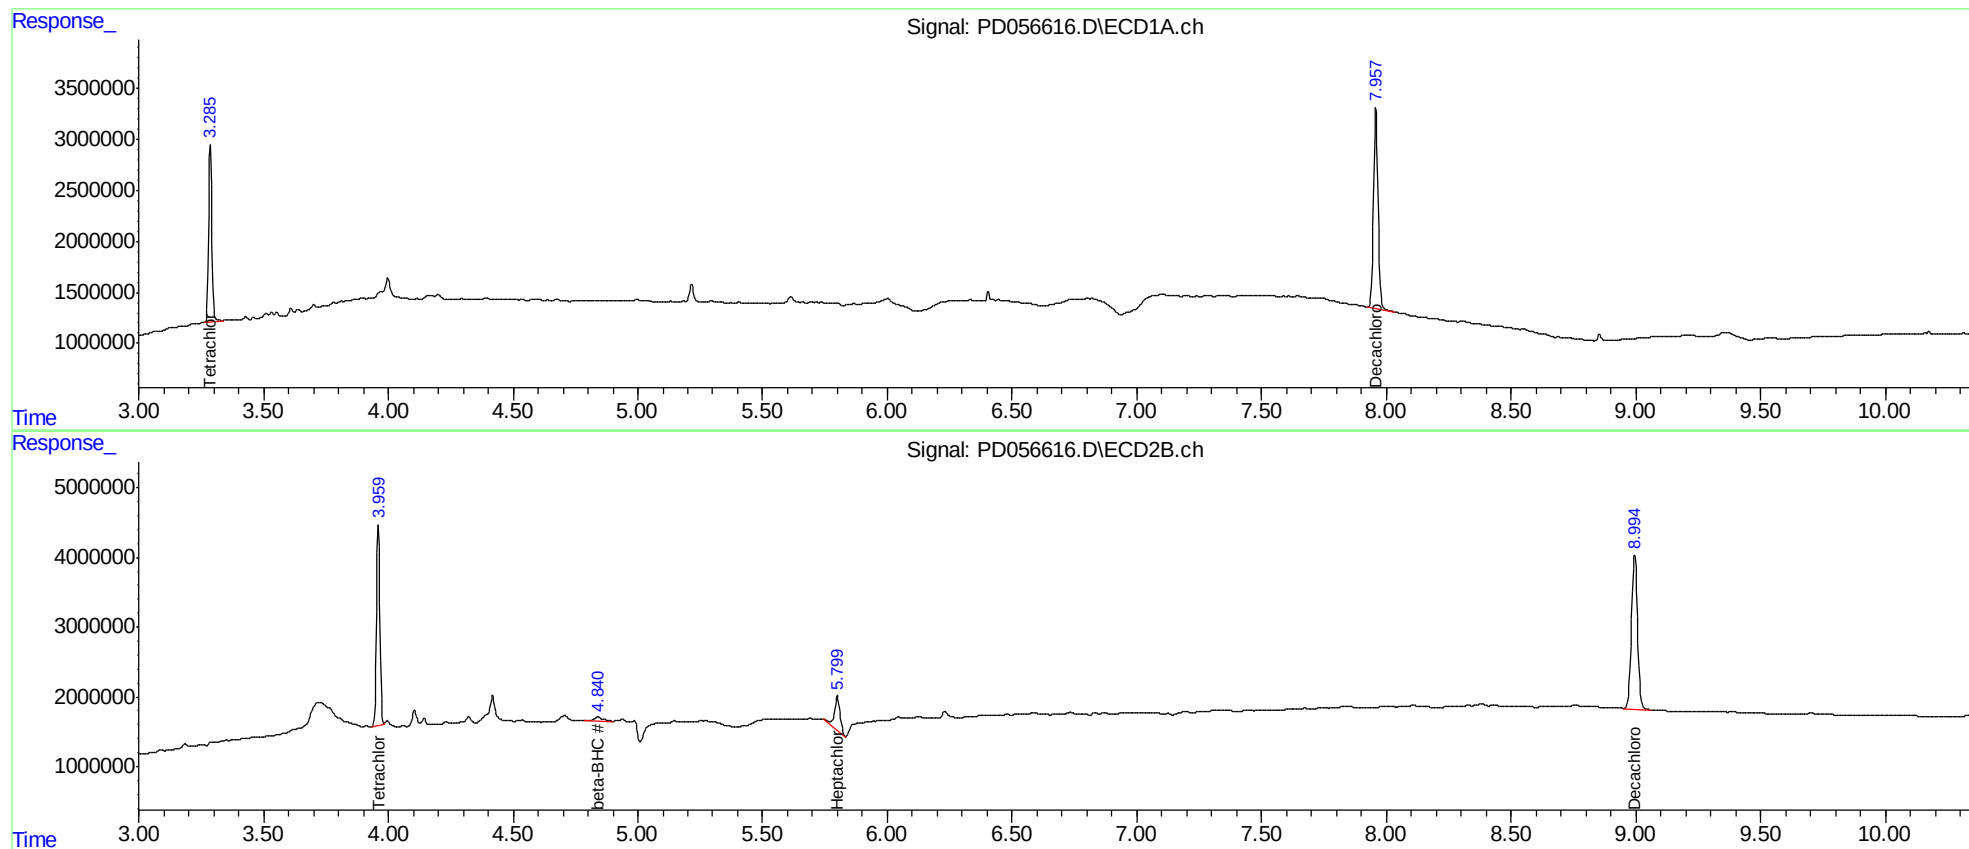


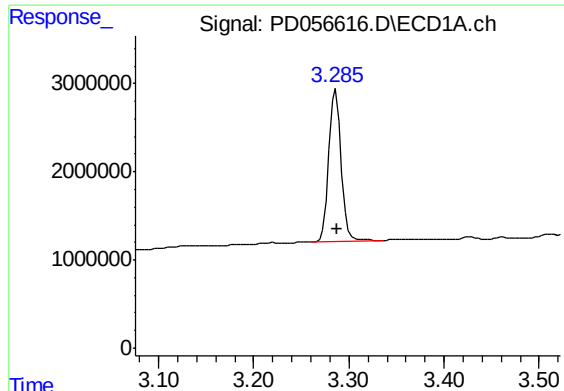

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: -0.002 min
Response: 15485937
Conc: 18.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0C75

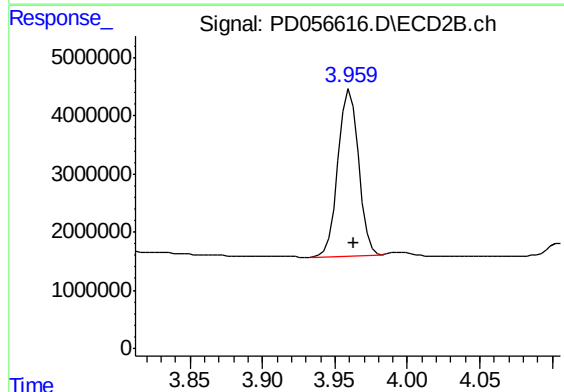


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.002 min
Response: 27955975
Conc: 23.25 ng/ml

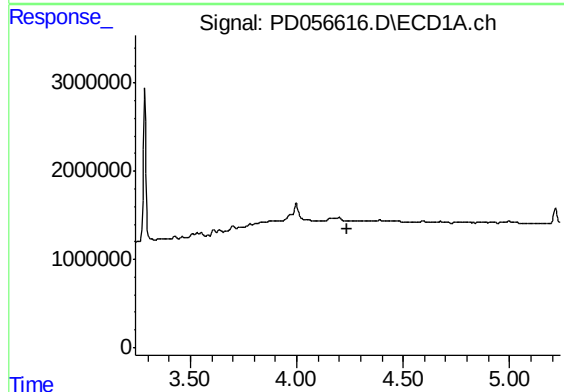


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

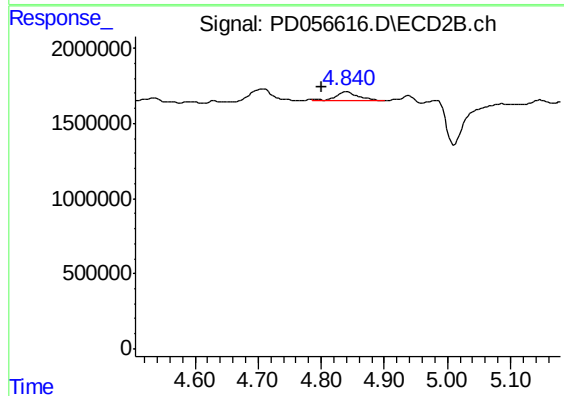

#6 beta-BHC


R.T.: 4.841 min
Delta R.T.: 0.040 min
Response: 1338378
Conc: 1.62 ng/ml

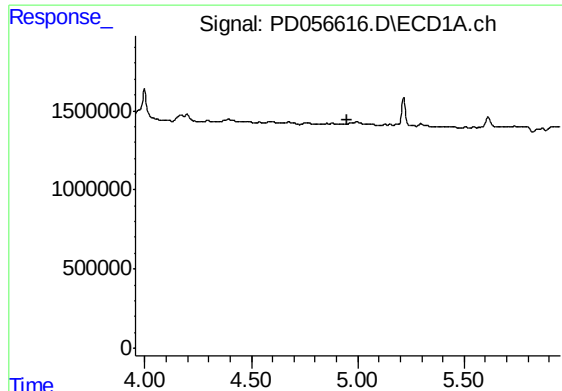

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0C75

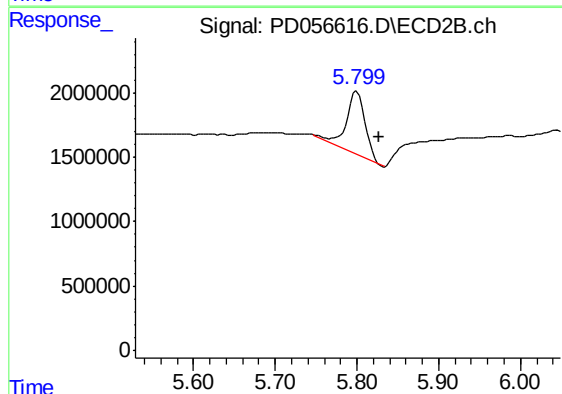


#8 Heptachlor epoxide

R.T.: 5.800 min
Delta R.T.: -0.027 min
Response: 7898632
Conc: 5.10 ng/ml

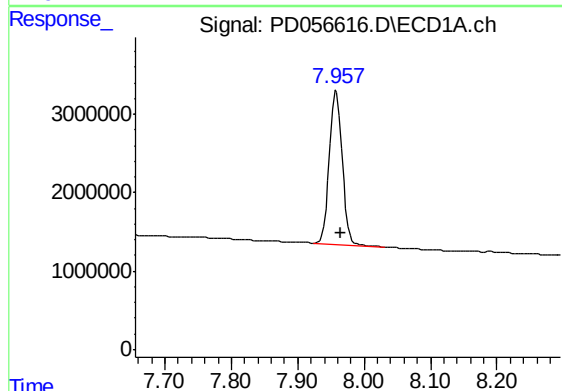

#27 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: -0.007 min
Response: 26128104
Conc: 28.94 ng/ml

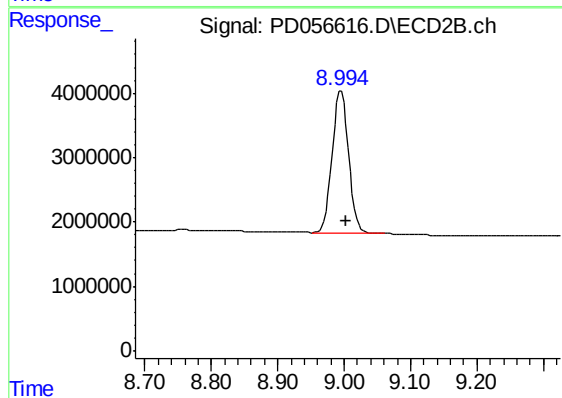

#27 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.007 min
Response: 38052245
Conc: 31.63 ng/ml