

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
 Data File : PD056620.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 14:18
 Operator : SG\AJ
 Sample : K6308-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BT4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 00:41:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	15963170	28851424	19.275	23.998
27)	SA Decachlor...	7.958	8.995	25708217	38159551	28.471	31.716
Target Compounds							
5)	MB Aldrin	0.000	5.457	0	704986	N.D.	0.429
10)	B trans-Chl...	0.000	6.051	0	1357655	N.D.	0.821


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
Data File : PD056620.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 14:18
Operator : SG\AJ
Sample : K6308-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0BT4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 00:41:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

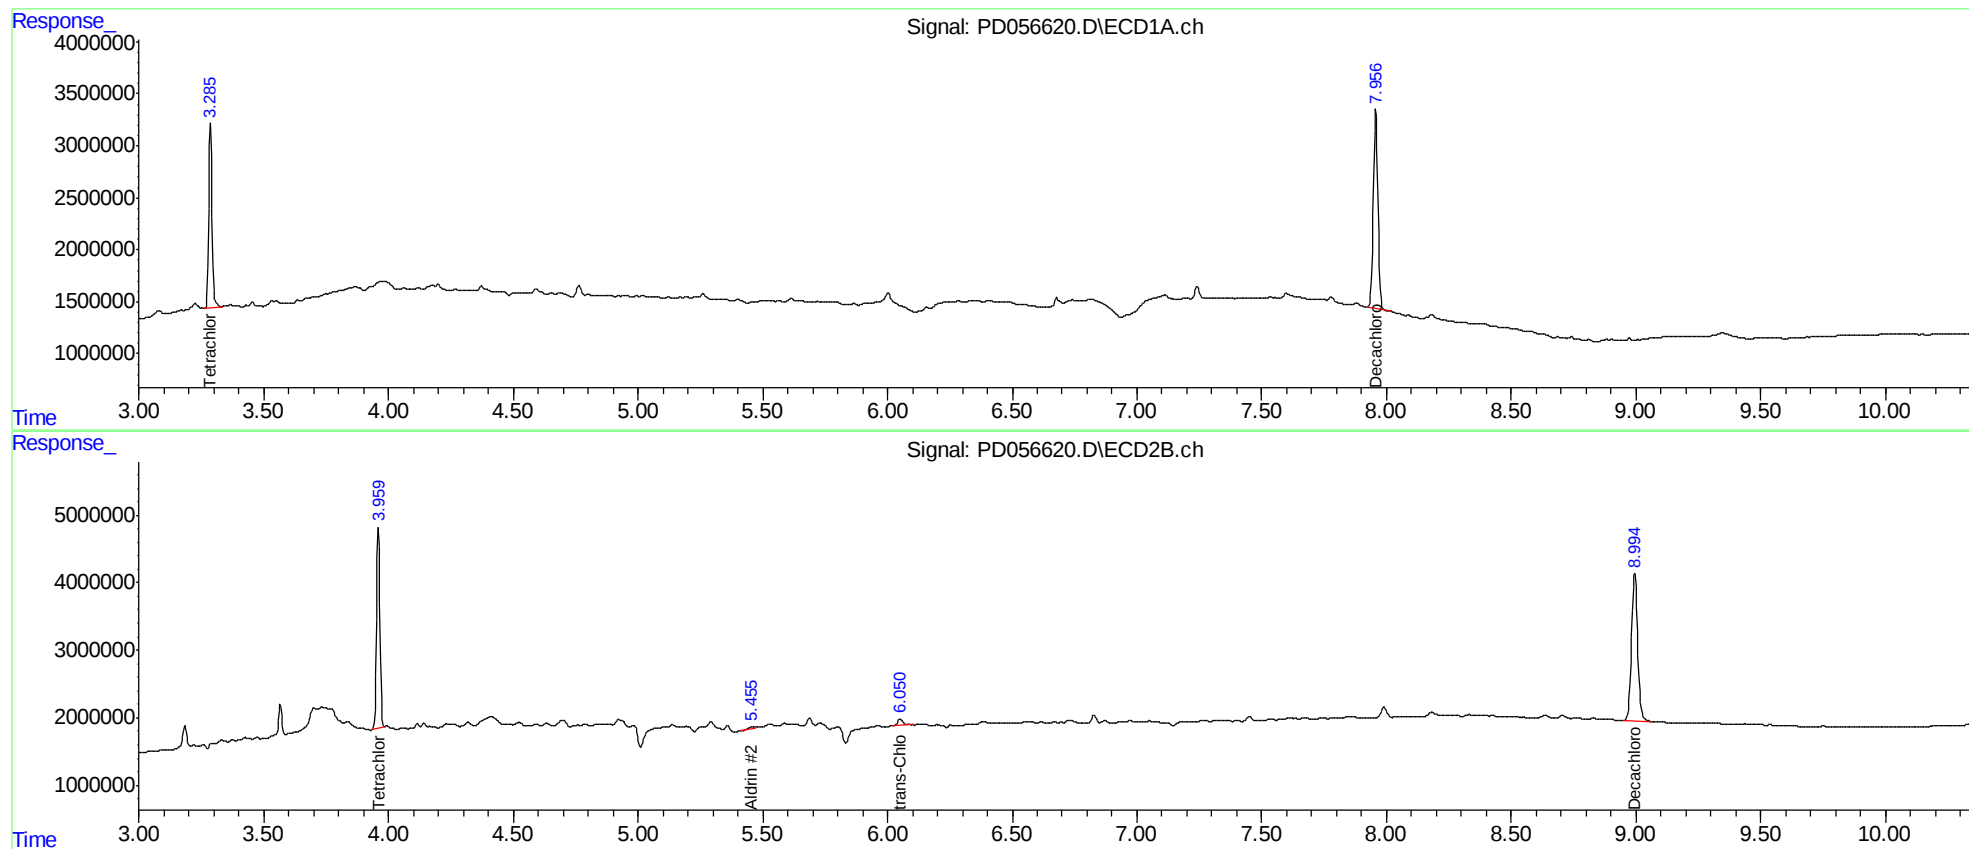


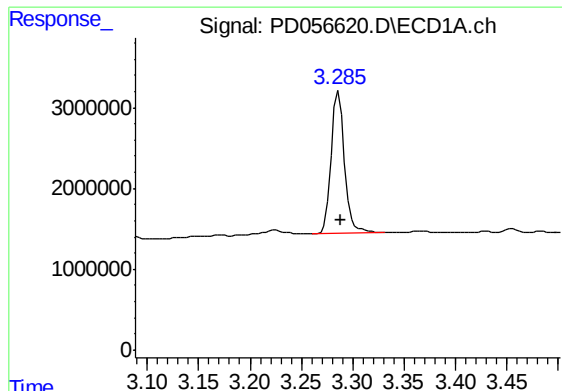

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: -0.002 min
Response: 15963170
Conc: 19.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BT4

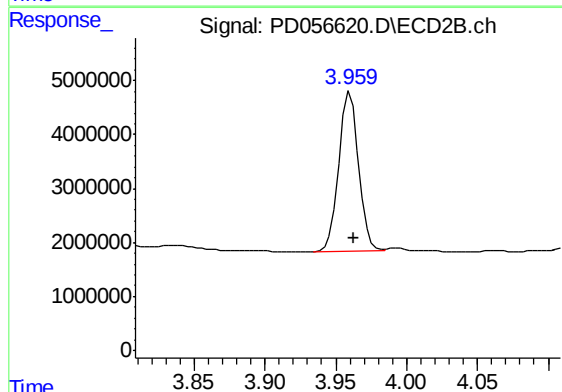


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.002 min
Response: 28851424
Conc: 24.00 ng/ml

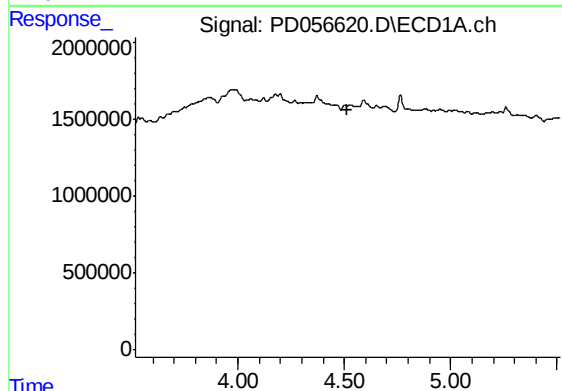


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.516 min
Response: 0
Conc: N.D.

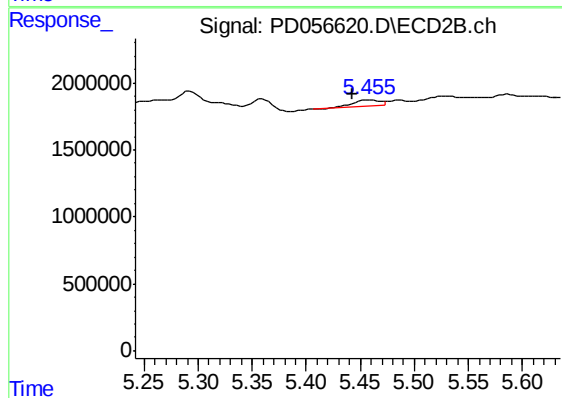

#5 Aldrin


R.T.: 5.457 min
Delta R.T.: 0.015 min
Response: 704986
Conc: 0.43 ng/ml

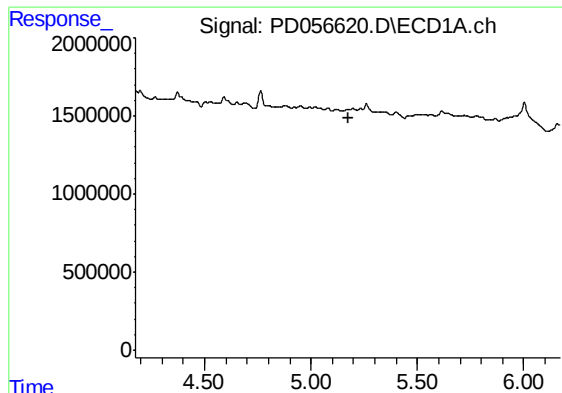

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BT4

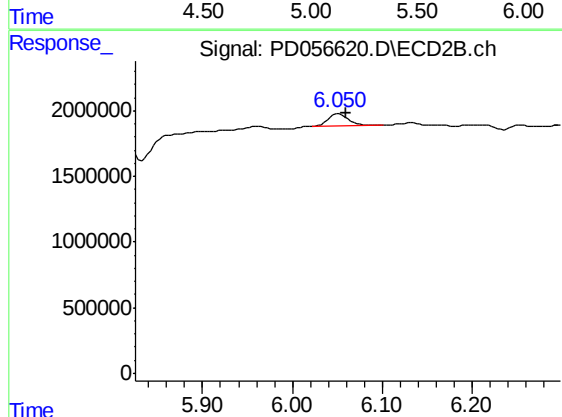


#10 trans-Chlordane

R.T.: 6.051 min
Delta R.T.: -0.009 min
Response: 1357655
Conc: 0.82 ng/ml

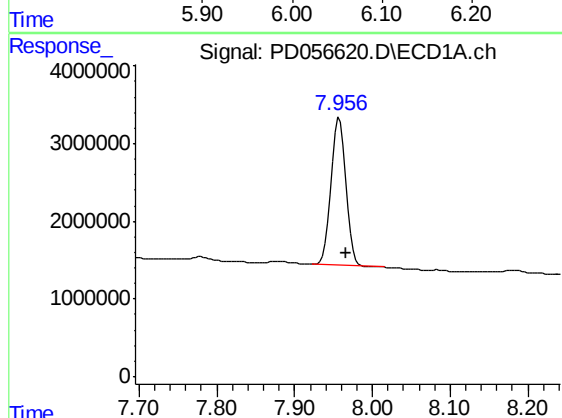

#27 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: -0.008 min
Response: 25708217
Conc: 28.47 ng/ml

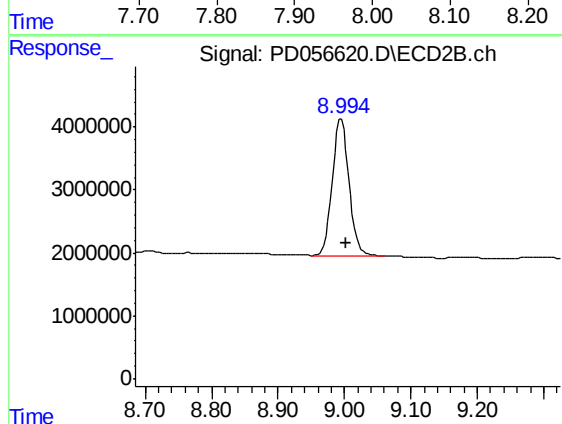

#27 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.007 min
Response: 38159551
Conc: 31.72 ng/ml