

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
 Data File : PD056633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 17:49
 Operator : SG\AJ
 Sample : K6314-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFF16

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 00:44:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	16643705	30674030	20.096	25.514 #
27)	SA Decachlor...	7.958	8.995	33389508	48567624	36.977	40.367
Target Compounds							
8)	B Heptachlo...	0.000	5.845	0	3630437	N.D.	2.343
10)	B trans-Chl...	0.000	6.003f	0	3452369	N.D.	2.088


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
Data File : PD056633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 17:49
Operator : SG\AJ
Sample : K6314-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFF16

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 00:44:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

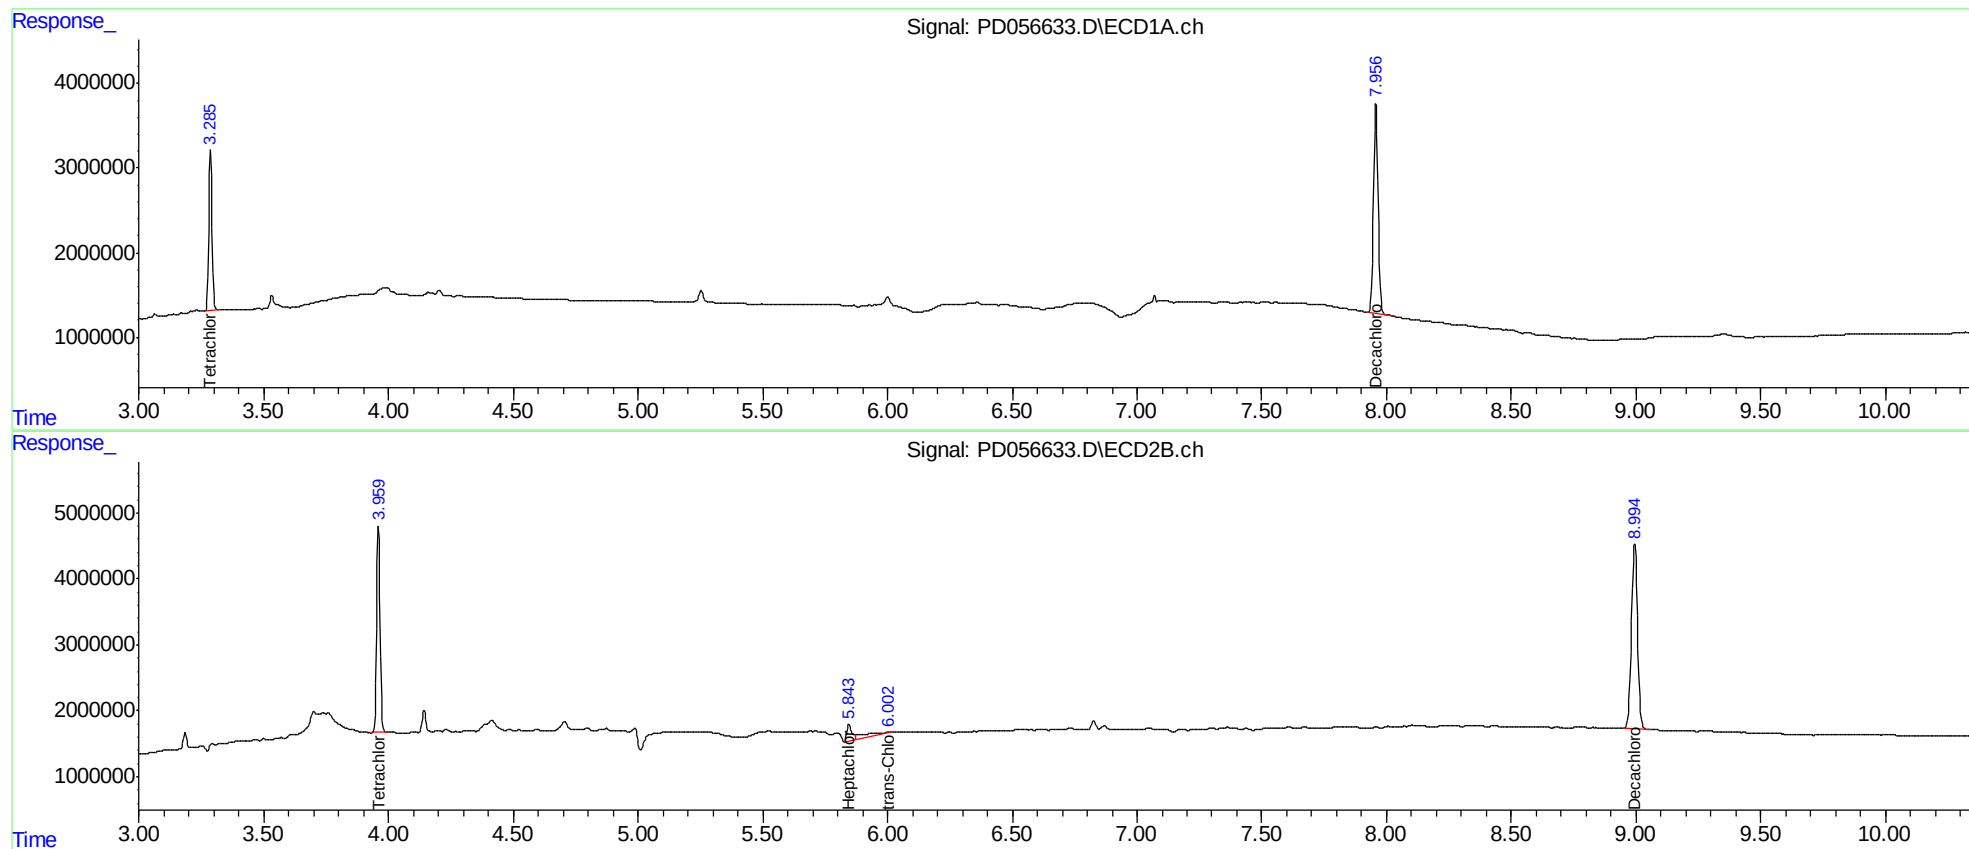


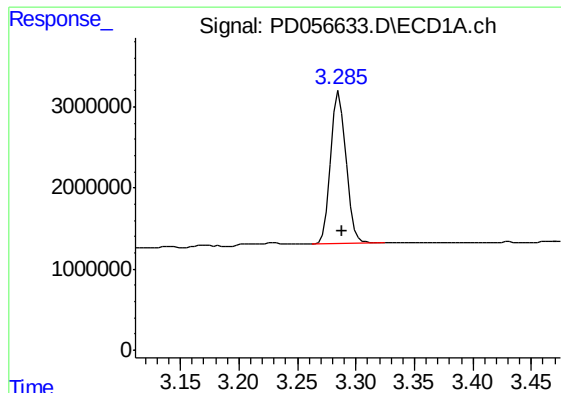

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: -0.002 min
Response: 16643705
Conc: 20.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFF16

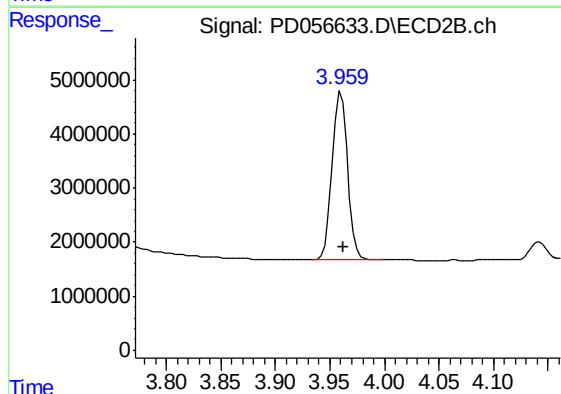


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.002 min
Response: 30674030
Conc: 25.51 ng/ml

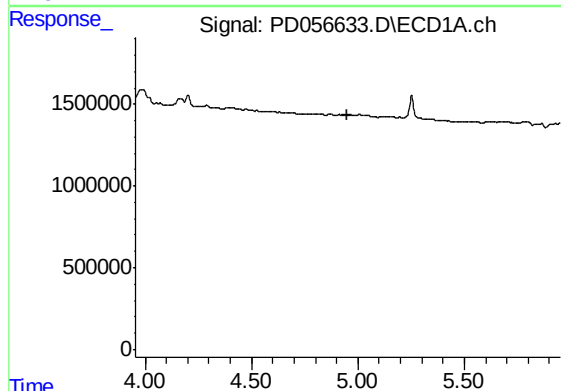


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

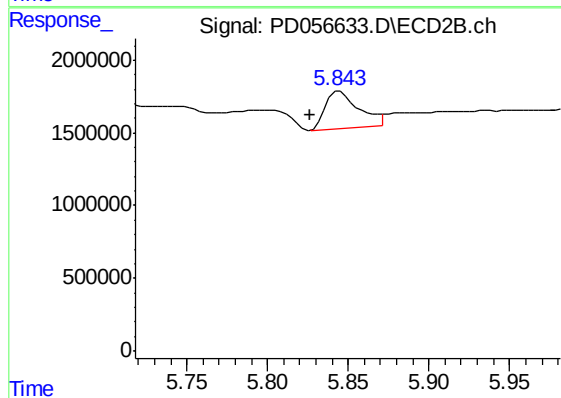

#8 Heptachlor epoxide


R.T.: 5.845 min
Delta R.T.: 0.018 min
Response: 3630437
Conc: 2.34 ng/ml

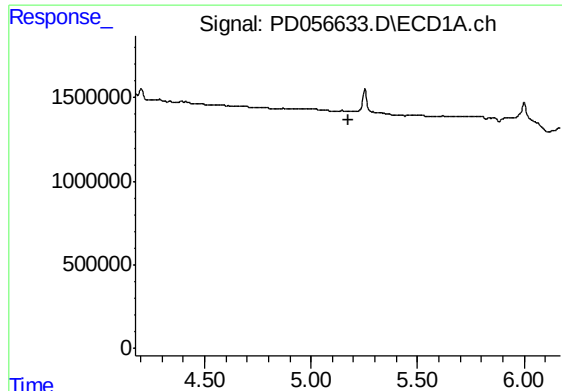

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFF16

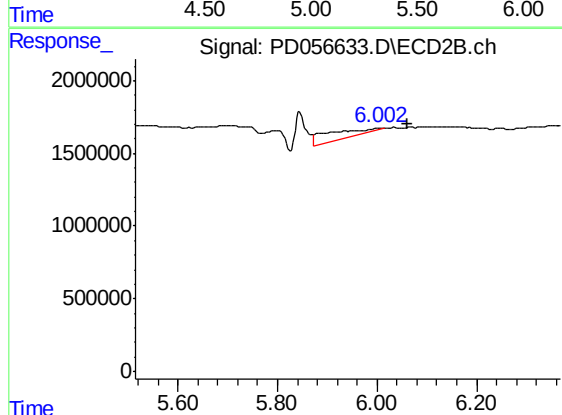


#10 trans-Chlordane

R.T.: 6.003 min
Delta R.T.: -0.057 min
Response: 3452369
Conc: 2.09 ng/ml

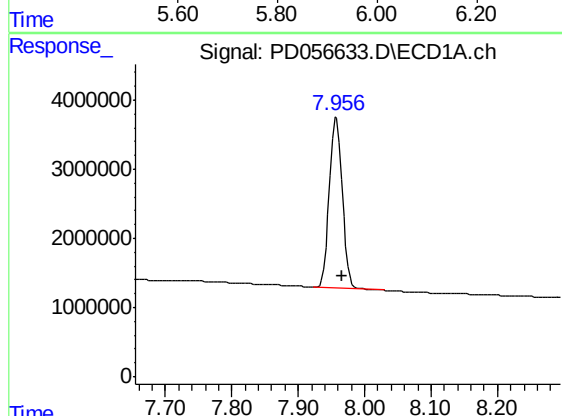

#27 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: -0.008 min
Response: 33389508
Conc: 36.98 ng/ml

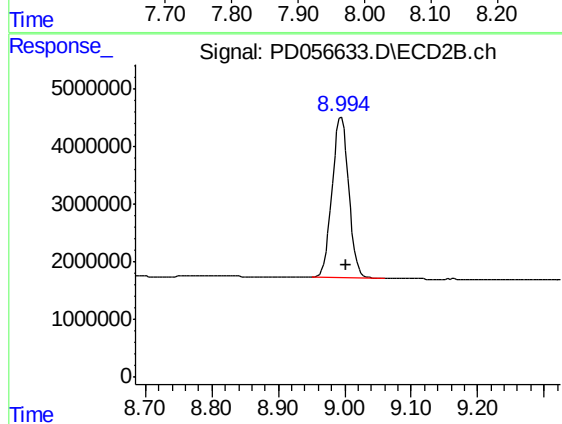

#27 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.008 min
Response: 48567624
Conc: 40.37 ng/ml