

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
 Data File : PD056637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 18:45
 Operator : SG\AJ
 Sample : K6314-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFF19

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 00:45:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	16310470	29881329	19.694	24.854 #
27)	SA Decachlor...	7.958	8.994	32174206	46152662	35.632	38.360
Target Compounds							
8)	B Heptachlo...	0.000	5.845	0	3532582	N.D.	2.280
10)	B trans-Chl...	0.000	6.006f	0	3726646	N.D.	2.254
13)	MA Dieldrin	0.000	6.434	0	555066	N.D.	0.353


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
Data File : PD056637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 18:45
Operator : SG\AJ
Sample : K6314-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFF19

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 00:45:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

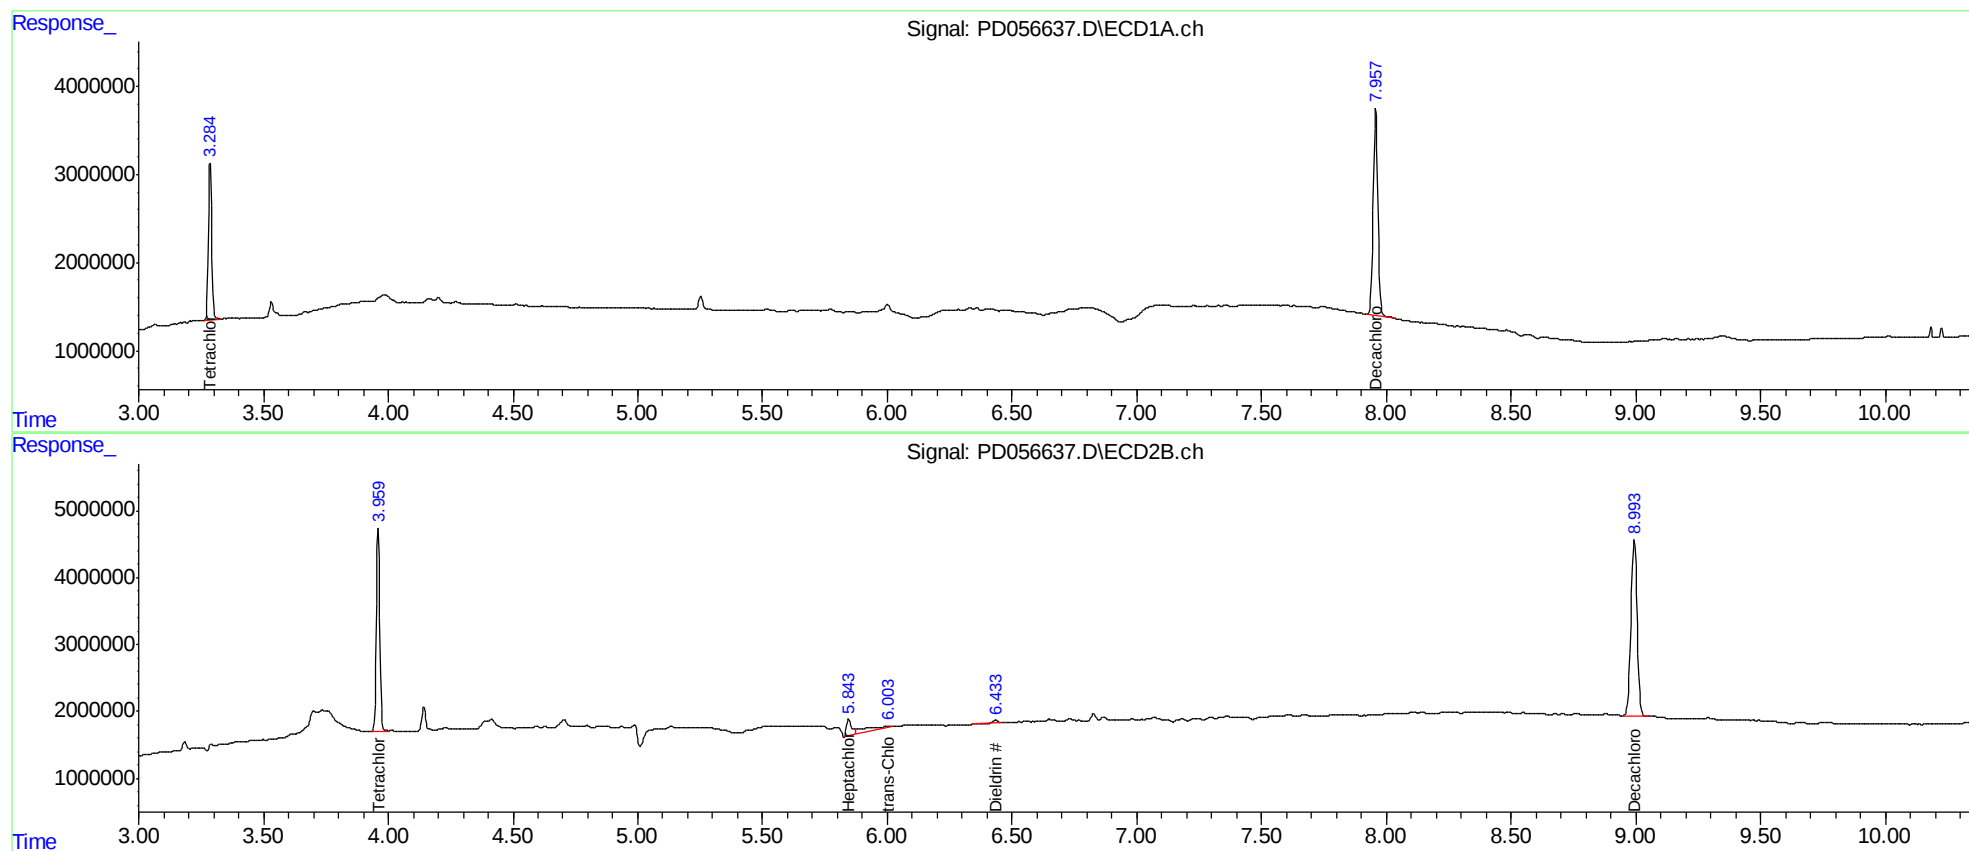


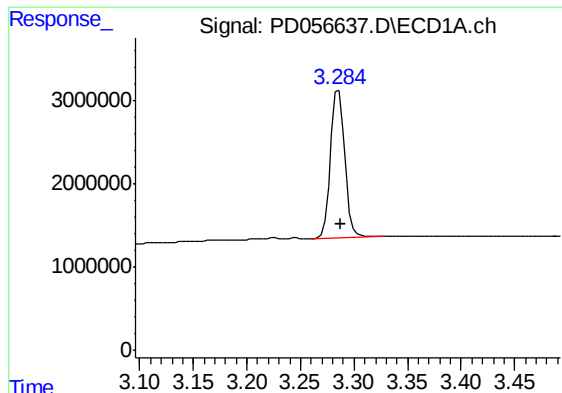

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: -0.002 min
Response: 16310470
Conc: 19.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFF19

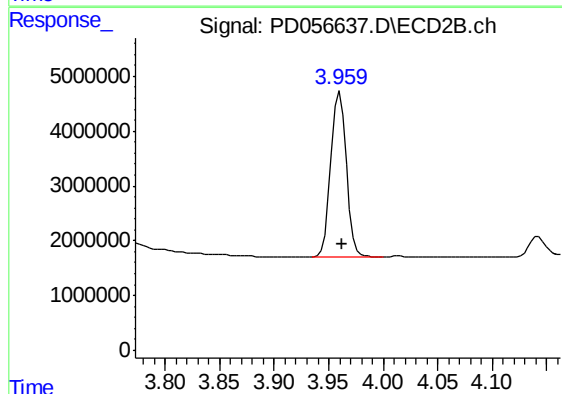


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.002 min
Response: 29881329
Conc: 24.85 ng/ml

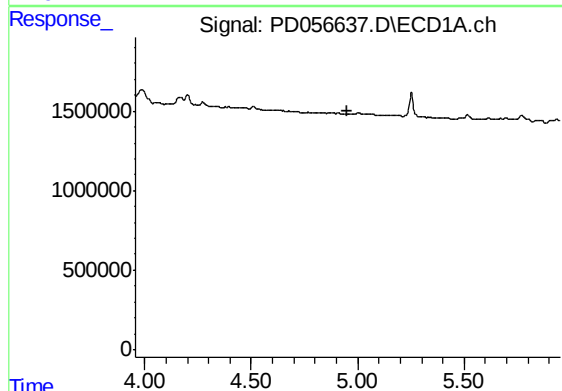


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

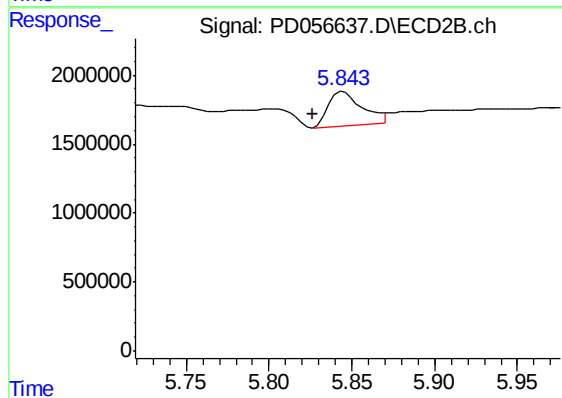

#8 Heptachlor epoxide


R.T.: 5.845 min
Delta R.T.: 0.018 min
Response: 3532582
Conc: 2.28 ng/ml

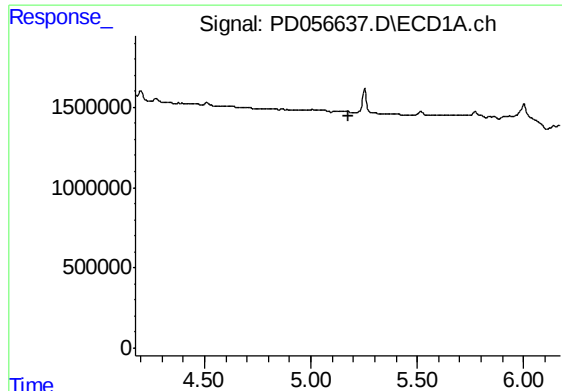

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFF19

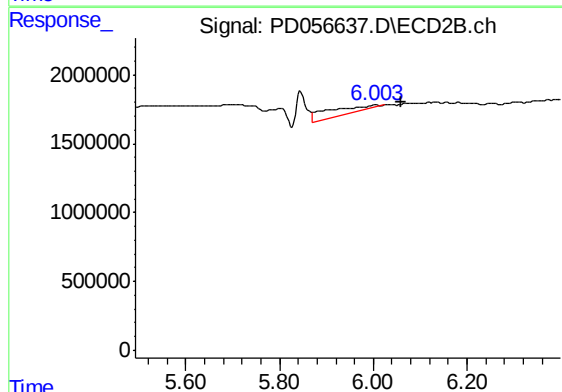


#10 trans-Chlordane

R.T.: 6.006 min
Delta R.T.: -0.054 min
Response: 3726646
Conc: 2.25 ng/ml

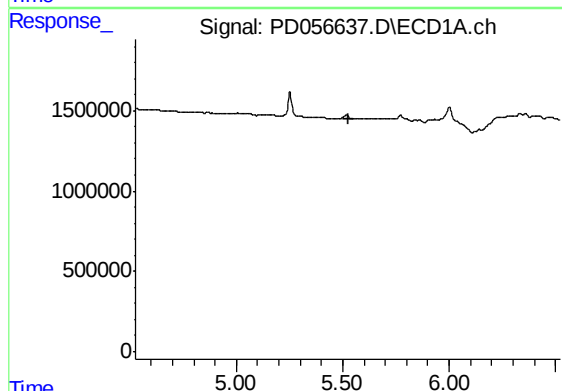


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

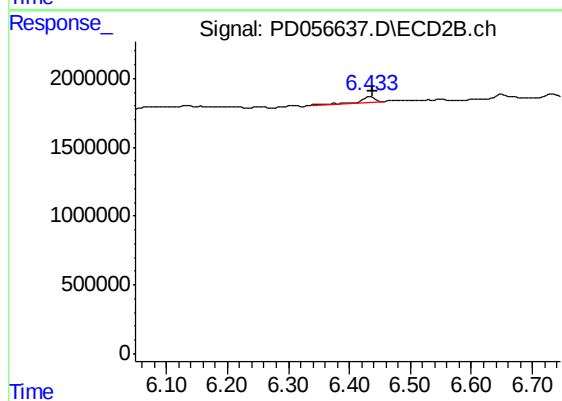

#13 Dieldrin


R.T.: 6.434 min
Delta R.T.: -0.004 min
Response: 555066
Conc: 0.35 ng/ml

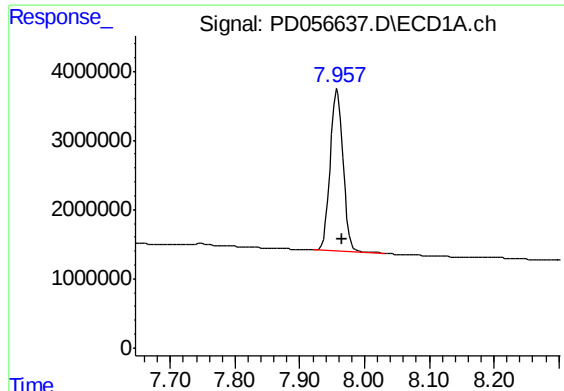

#27 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: -0.007 min
Response: 32174206
Conc: 35.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFF19

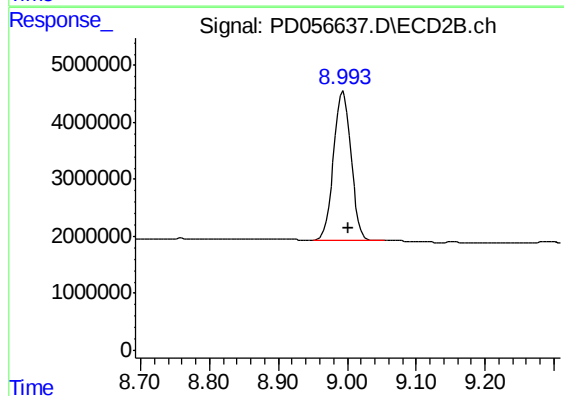

#27 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: -0.008 min
Response: 46152662
Conc: 38.36 ng/ml