

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
 Data File : PD056640.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 19:28
 Operator : SG\AJ
 Sample : K6314-11
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFF14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 00:46:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	16460123	29907241	19.875	24.876 #
27)	SA Decachlor...	7.956	8.993	30711569	44730645	34.012	37.178
Target Compounds							
8)	B Heptachlo...	0.000	5.852	0	13257480	N.D.	8.557
9)	A Endosulfan I	5.250	0.000	477291	0	0.516	N.D. #
10)	B trans-Chl...	5.233f	0.000	1568305	0	1.496	N.D. #
11)	B cis-Chlor...	5.233	0.000	1568305	0	1.536	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
Data File : PD056640.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 19:28
Operator : SG\AJ
Sample : K6314-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFF14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 00:46:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

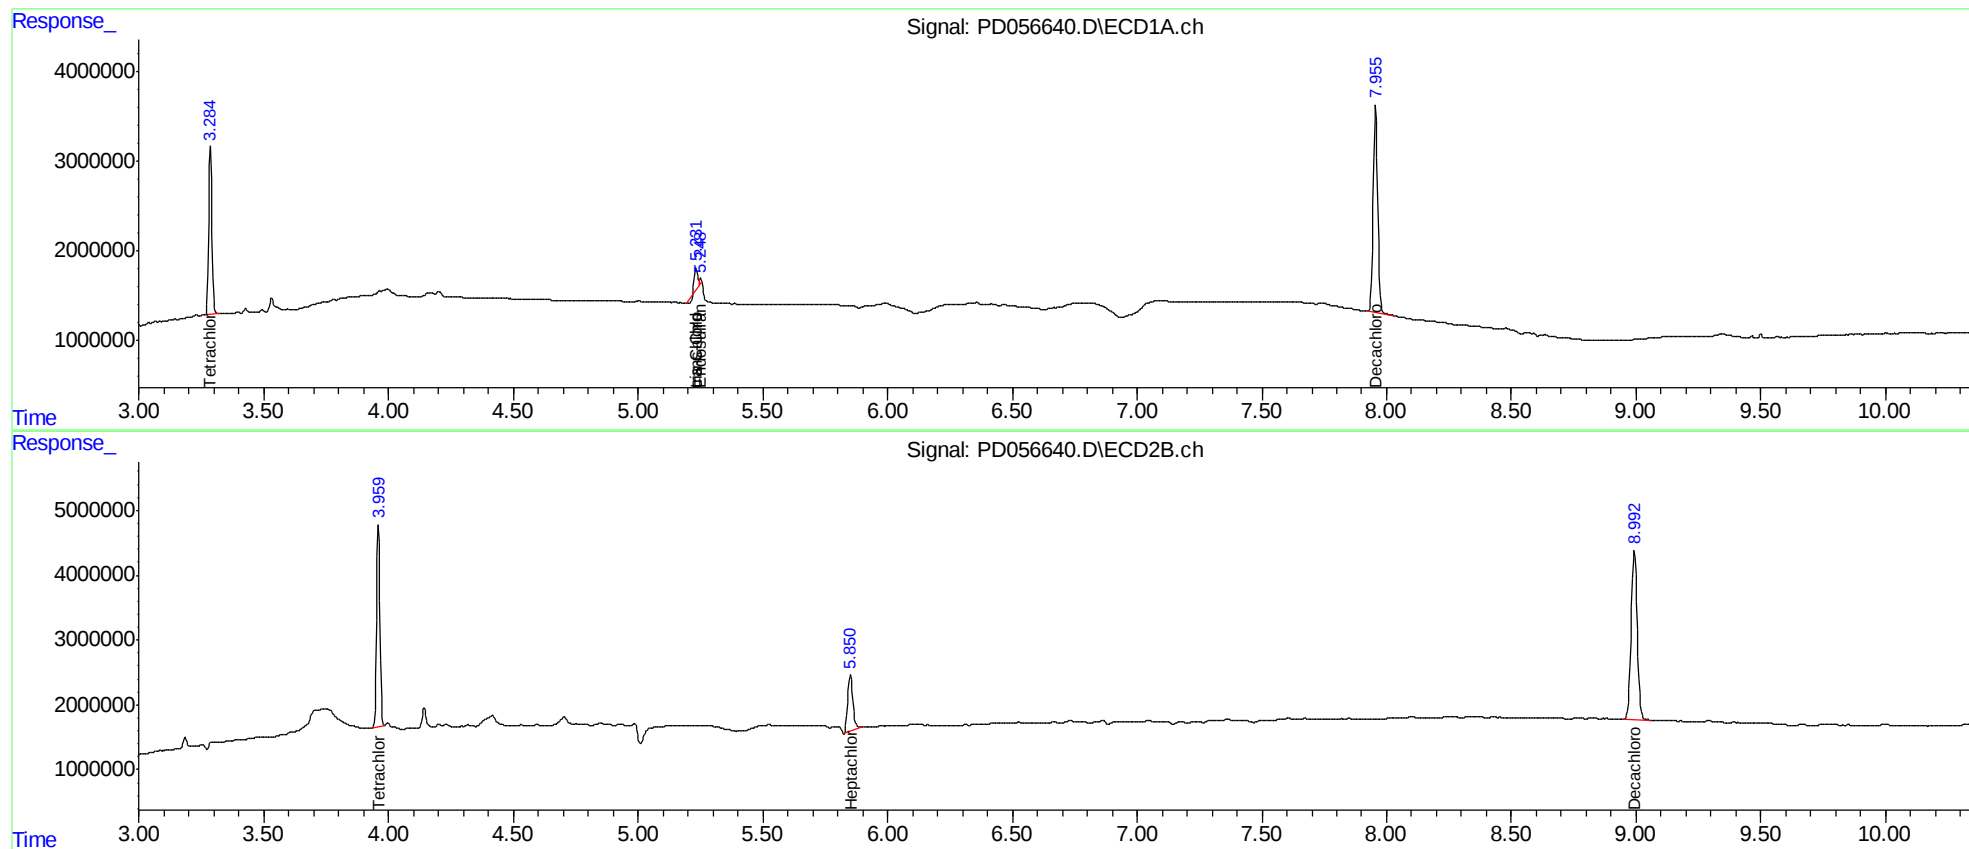


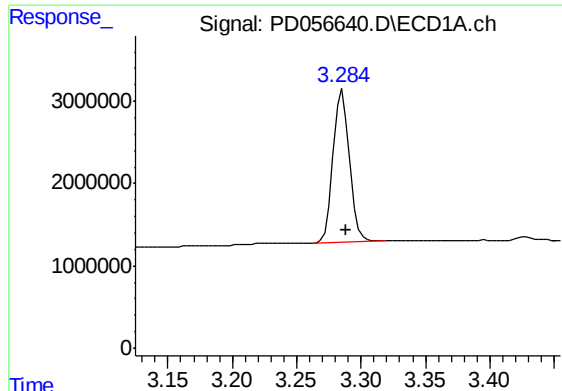

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: -0.002 min
Response: 16460123
Conc: 19.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFF14

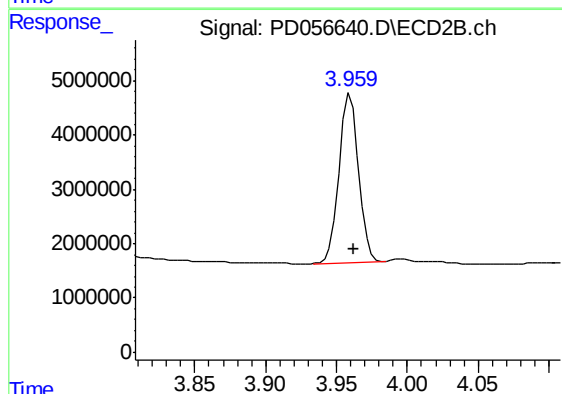


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.003 min
Response: 29907241
Conc: 24.88 ng/ml

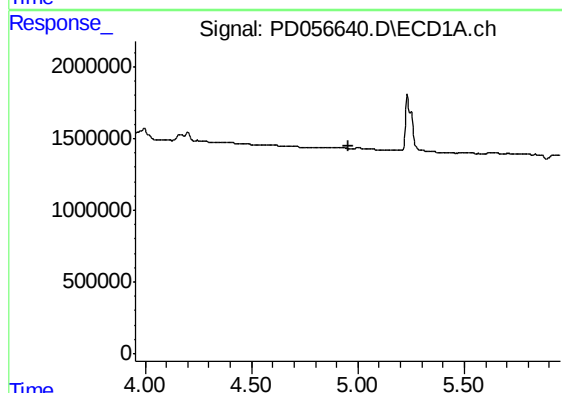


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

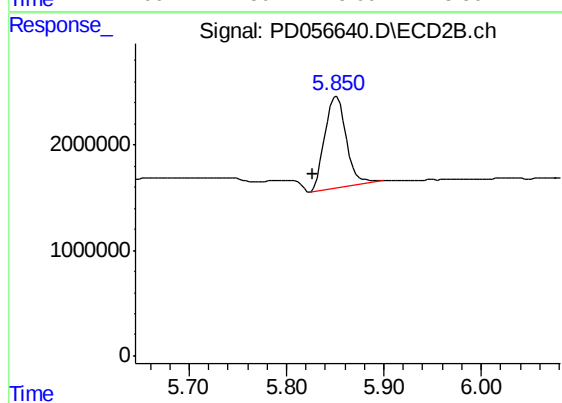

#8 Heptachlor epoxide


R.T.: 5.852 min
Delta R.T.: 0.025 min
Response: 13257480
Conc: 8.56 ng/ml

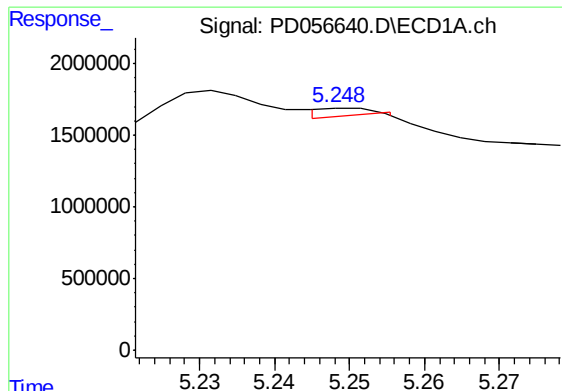

#9 Endosulfan I


R.T.: 5.250 min
Delta R.T.: -0.034 min
Response: 477291
Conc: 0.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFF14

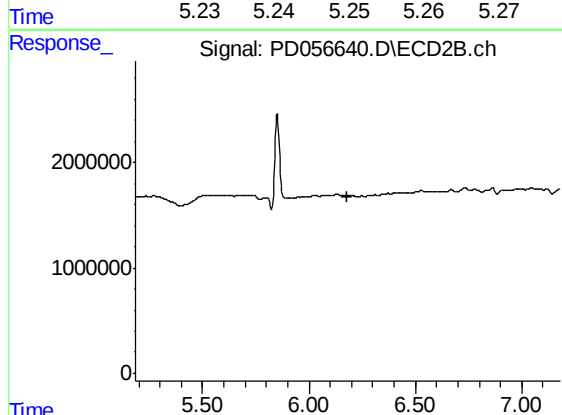


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.182 min
Response: 0
Conc: N.D.

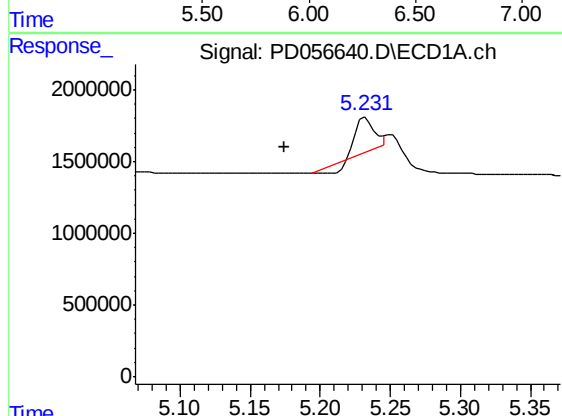


#10 trans-Chlordane

R.T.: 5.233 min
Delta R.T.: 0.058 min
Response: 1568305
Conc: 1.50 ng/ml

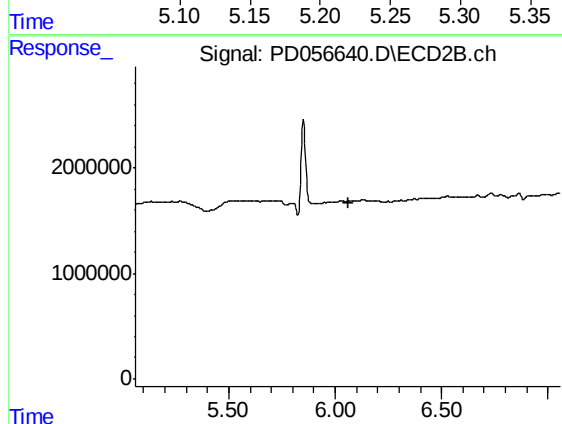

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.060 min
Response: 0
Conc: N.D.

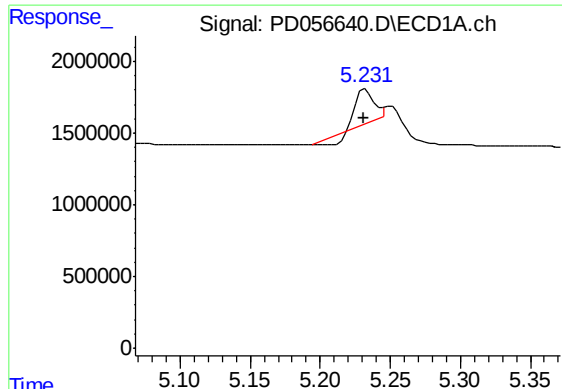

#11 cis-Chlordane


R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 1568305
Conc: 1.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFF14

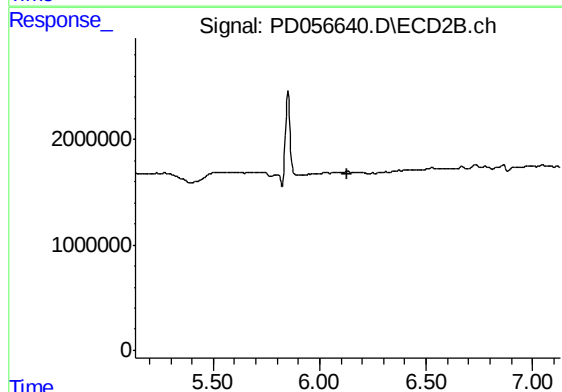


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.132 min
Response: 0
Conc: N.D.

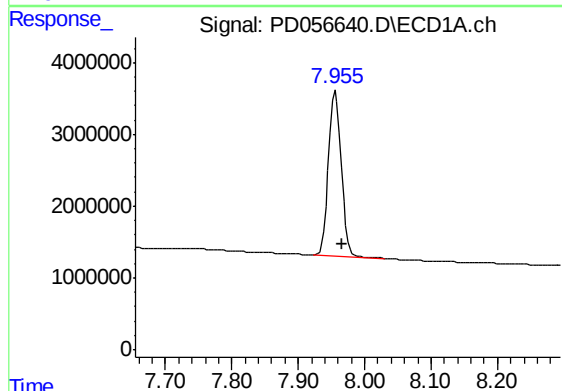

#27 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: -0.009 min
Response: 30711569
Conc: 34.01 ng/ml

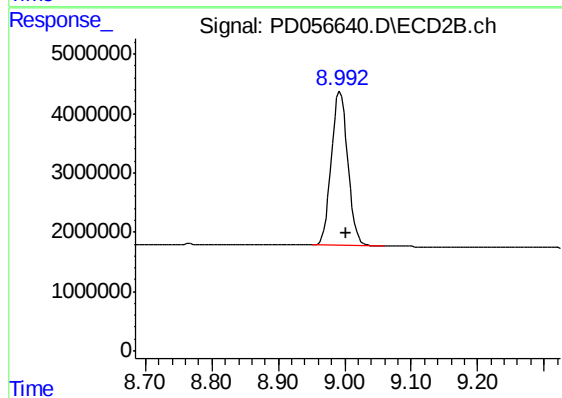

#27 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: -0.009 min
Response: 44730645
Conc: 37.18 ng/ml