

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
 Data File : PD056648.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 21:20
 Operator : SG\AJ
 Sample : K6254-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0C21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 00:48:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	10890211	19679441	13.149	16.369
27)	SA Decachlor...	7.958	8.995	22366418	31590896	24.770	26.257
Target Compounds							
15)	B Endosulfa...	0.000	6.872	0	1471430	N.D.	1.004


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
Data File : PD056648.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 21:20
Operator : SG\AJ
Sample : K6254-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0C21

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 00:48:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

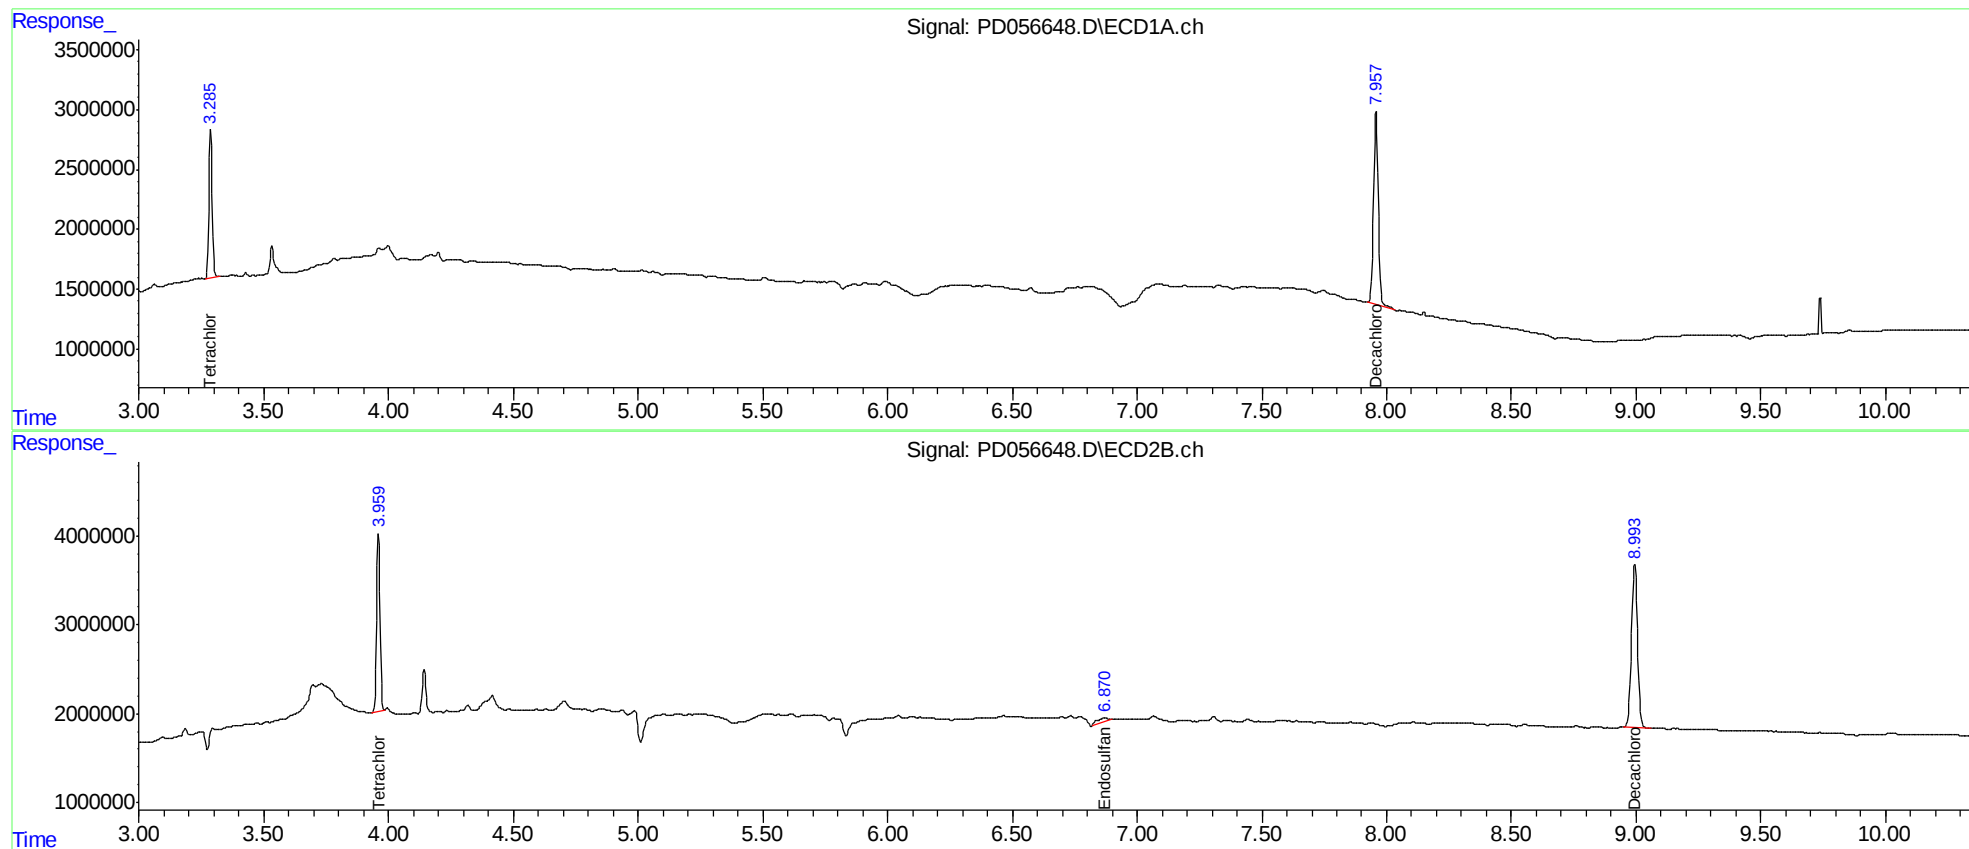


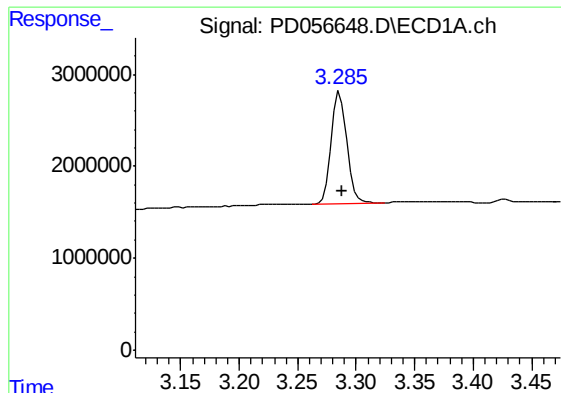

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: -0.002 min
Response: 10890211
Conc: 13.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0C21

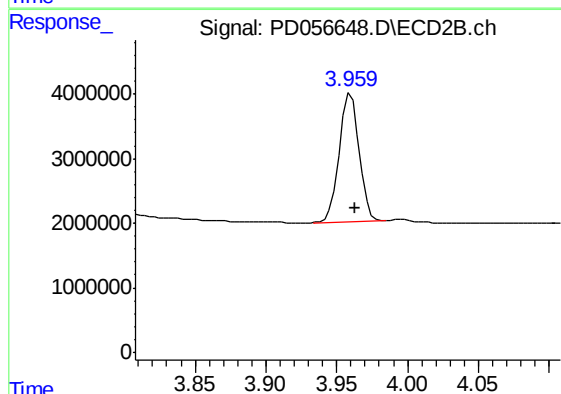


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.002 min
Response: 19679441
Conc: 16.37 ng/ml

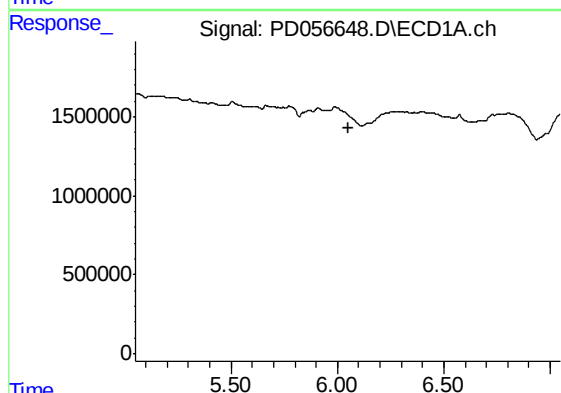


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.051 min
Response: 0
Conc: N.D.

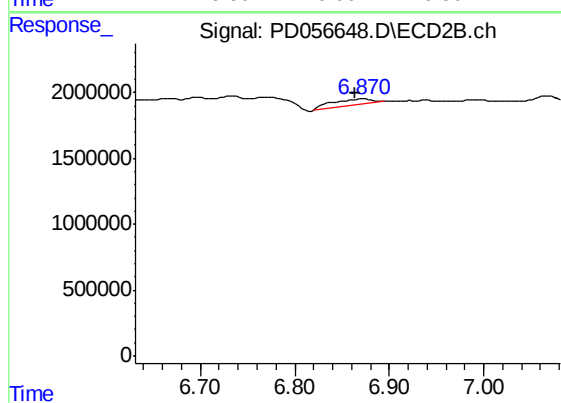

#15 Endosulfan II


R.T.: 6.872 min
Delta R.T.: 0.008 min
Response: 1471430
Conc: 1.00 ng/ml

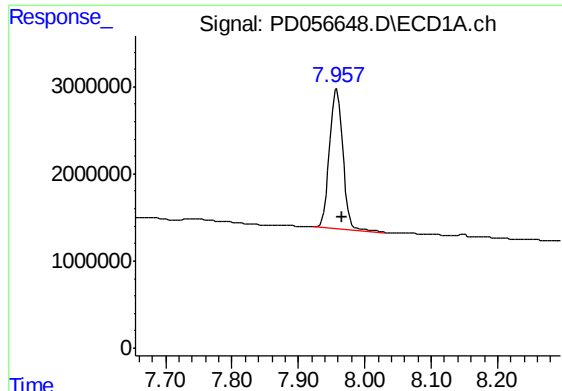

#27 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: -0.007 min
Response: 22366418
Conc: 24.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0C21

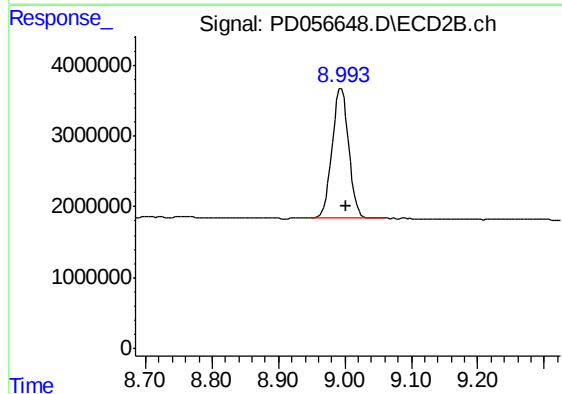

#27 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.008 min
Response: 31590896
Conc: 26.26 ng/ml