

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
 Data File : PD056657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2019 23:26
 Operator : SG\AJ
 Sample : K6238-04
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFPZ7

Manual Integrations
 APPROVED

Ankita
 12/20/2019 10:54:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 03:29:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	4257699	9367193	5.141	7.791 #
2)	SA Decachlor...	7.956	8.992	6612829	8702896	7.323	7.233m
Target Compounds							
10)	B trans-Chl...	5.168	6.047	752129	3625170	0.717m	2.193m#
11)	B cis-Chlor...	5.225	6.129	1128611	2728934	1.105m	1.693 #
12)	B 4,4'-DDE	5.394	6.281	829231	1837255	0.821m	1.170 #
16)	A 4,4'-DDD	5.909	6.770	502267	1371897	0.706m	1.166m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121919\
Data File : PD056657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2019 23:26
Operator : SG\AJ
Sample : K6238-04
Misc :
ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 03:29:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

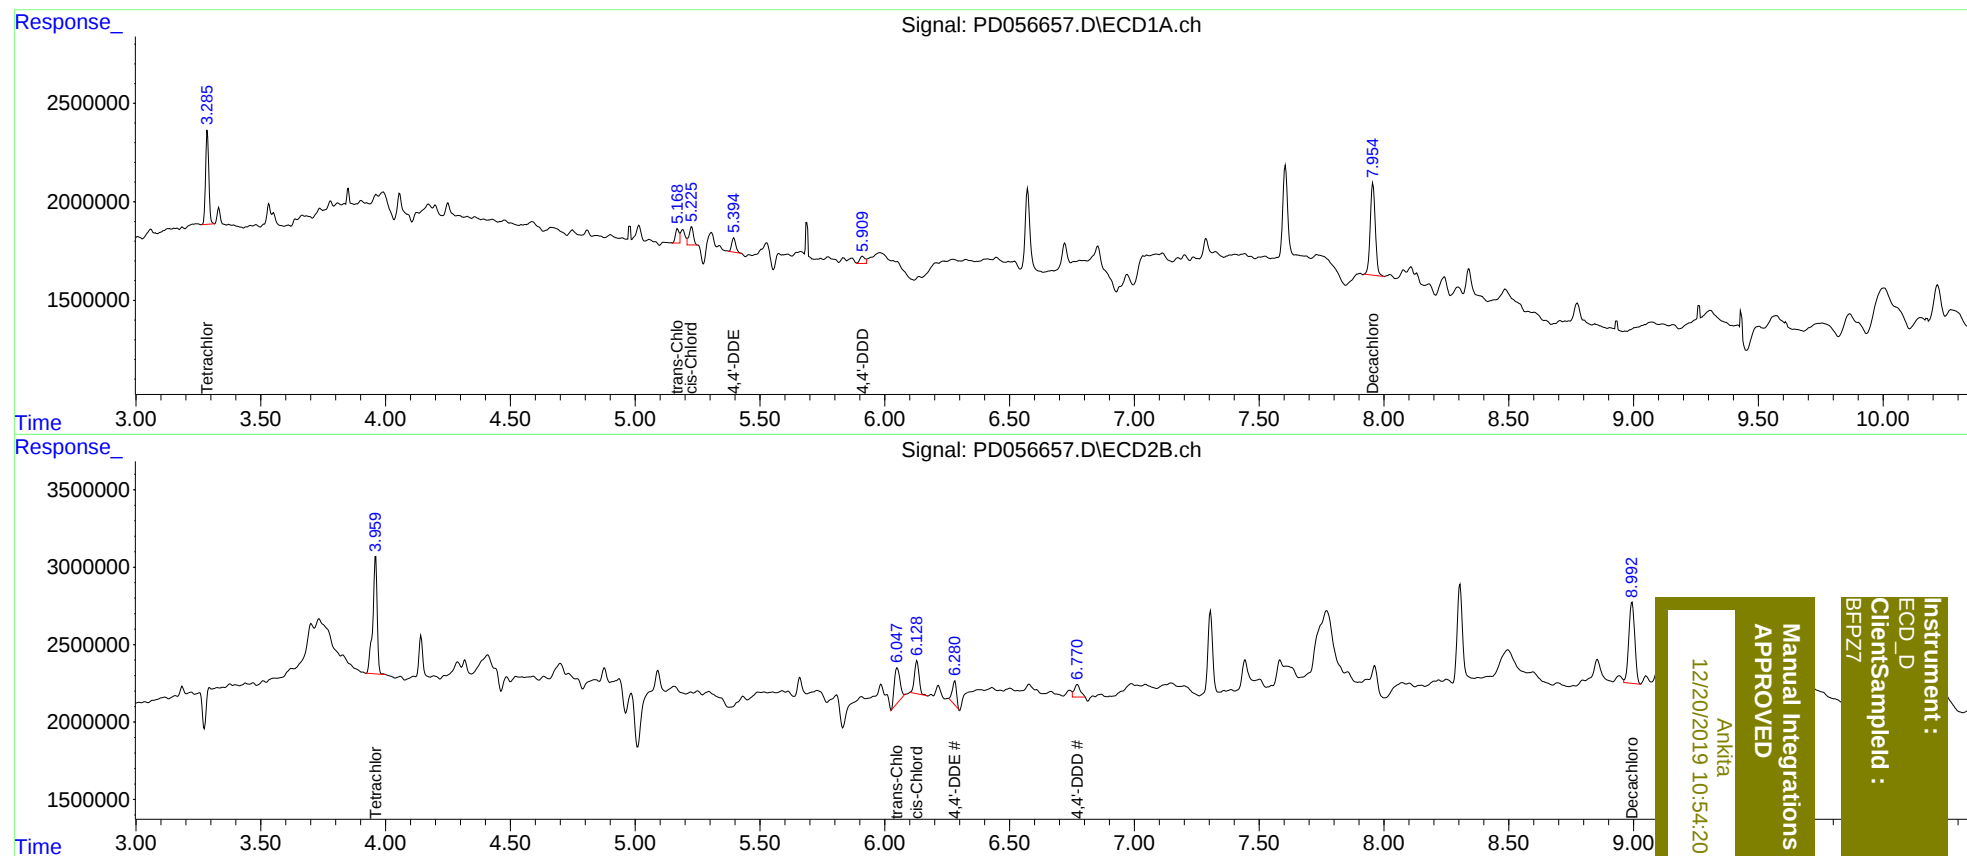

12/20/2019 10:54:20 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sample :
BFPZ7