

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121922\
 Data File : PD073359.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2022 15:55
 Operator : AR\AJ
 Sample : N6103-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TT-210-IDWSO-20221215

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 20:25:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 16 15:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.700	3.458	24137211	1080.1E6	11.517	10.982
28)	SA Decachlor...	7.825	8.907	36542531	288.5E6	15.093	16.367

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121922\
Data File : PD073359.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2022 15:55
Operator : AR\AJ
Sample : N6103-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TT-210-IDWSO-20221215

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 20:25:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
Quant Title : GC Extractables
QLast Update : Fri Dec 16 15:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

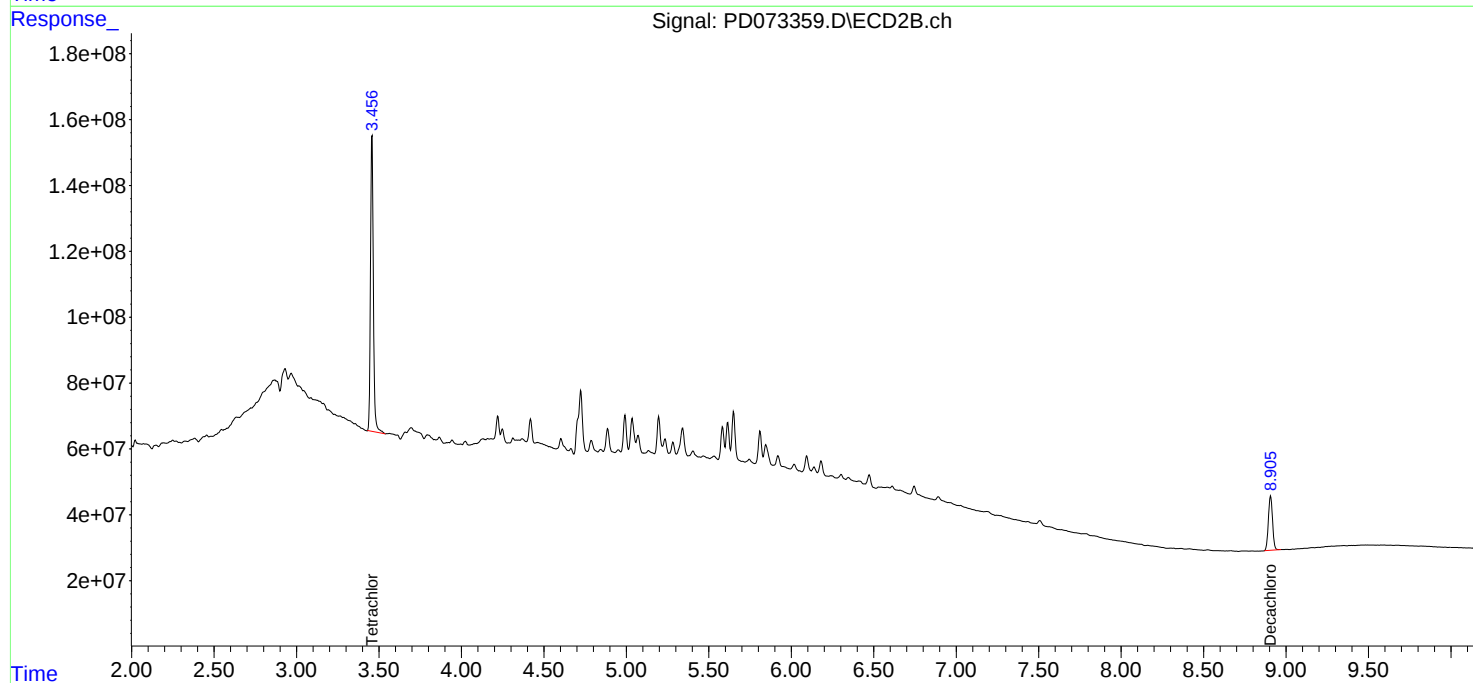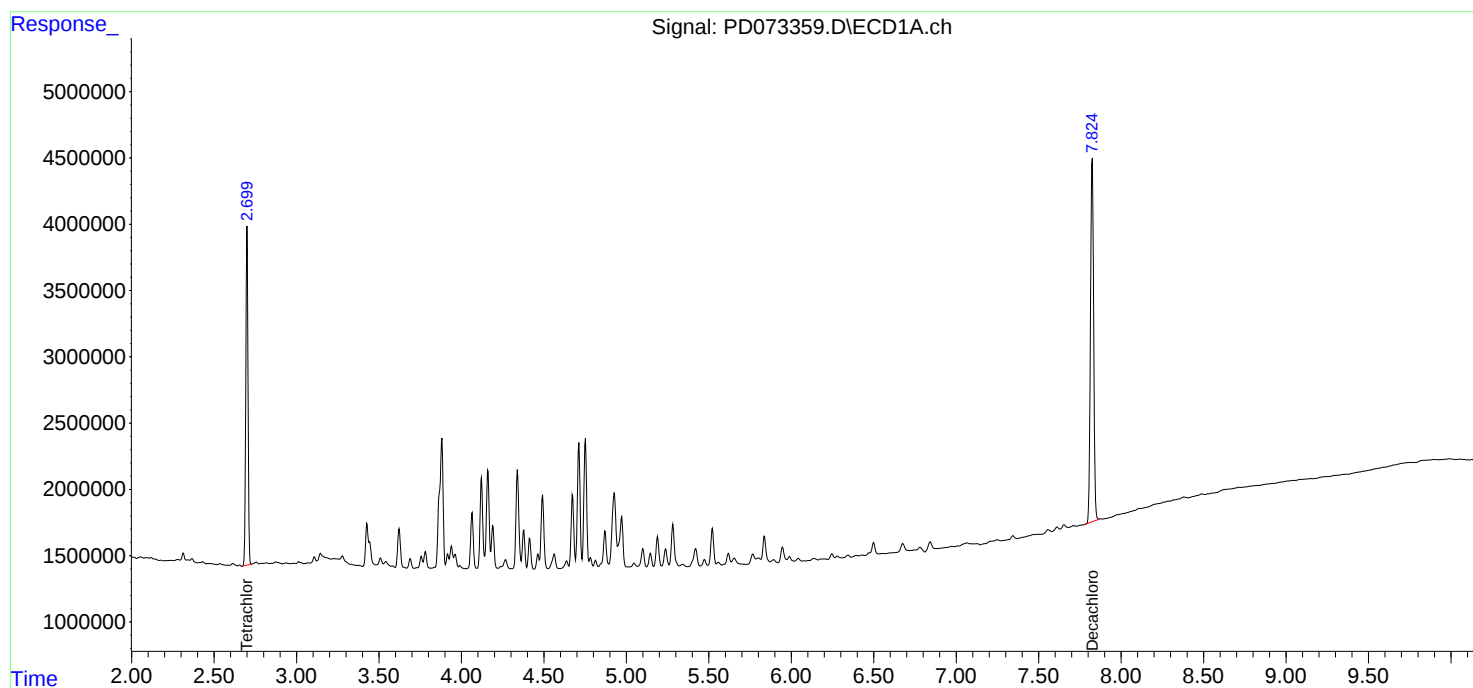


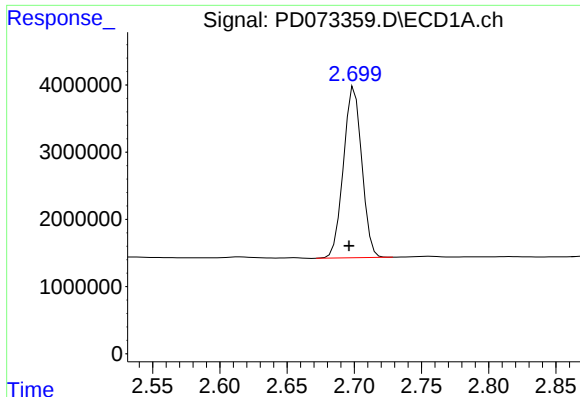

#1 Tetrachloro-m-xylene


R.T.: 2.700 min
Delta R.T.: 0.004 min
Response: 24137211
Conc: 11.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
TT-210-IDWSO-20221215

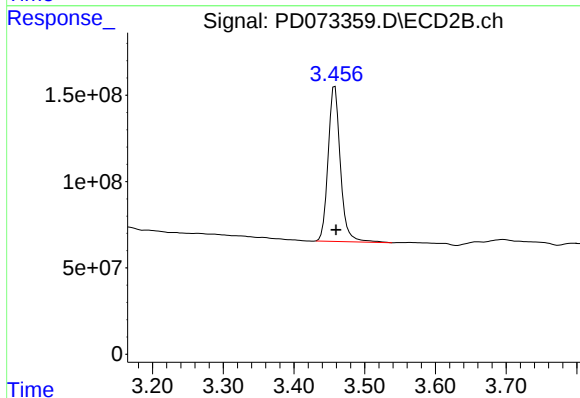


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: -0.001 min
Response: 1080080644
Conc: 10.98 ng/ml

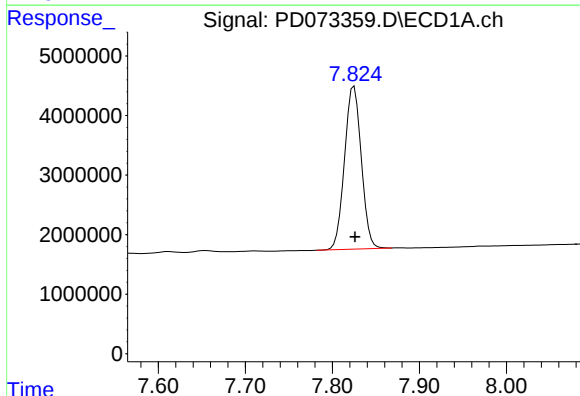

#28 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: -0.001 min
Response: 36542531
Conc: 15.09 ng/ml

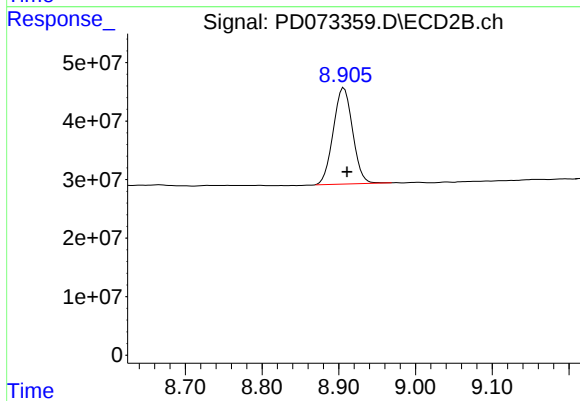

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: -0.004 min
Response: 288503529
Conc: 16.37 ng/ml