
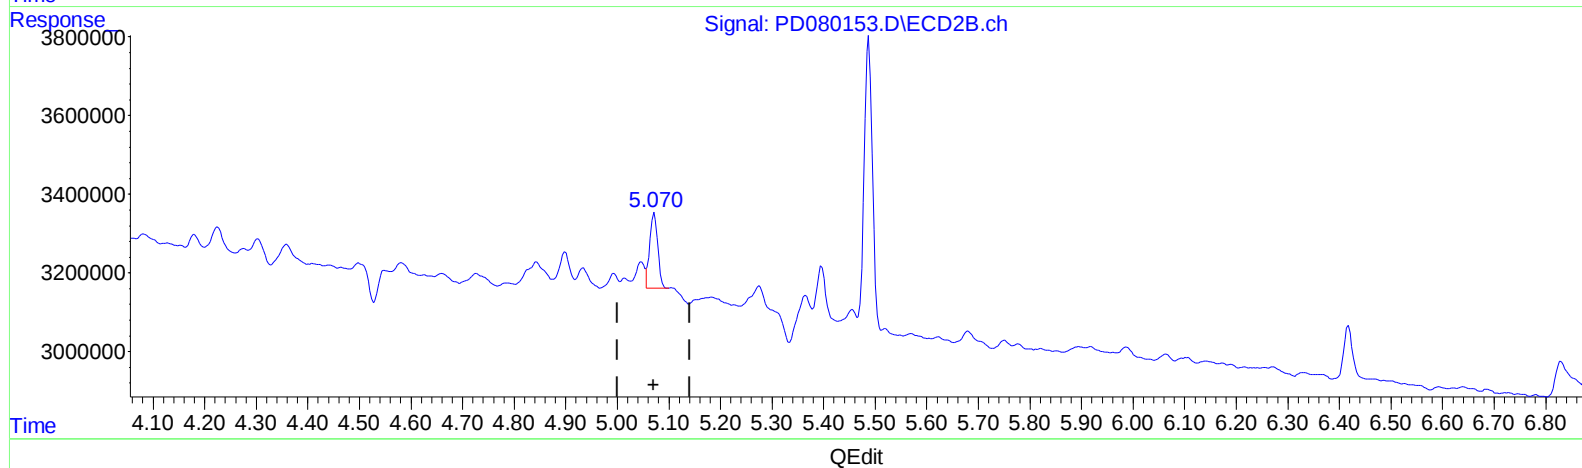


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD121923\  
Data File : PD080153.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 17 Dec 2023 14:54  
Operator : AR\AJ  
Sample : 05794-04  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 17 20:55:33 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121623CLP.M  
Quant Title : GC Extractables  
QLast Update : Sat Dec 16 03:10:23 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

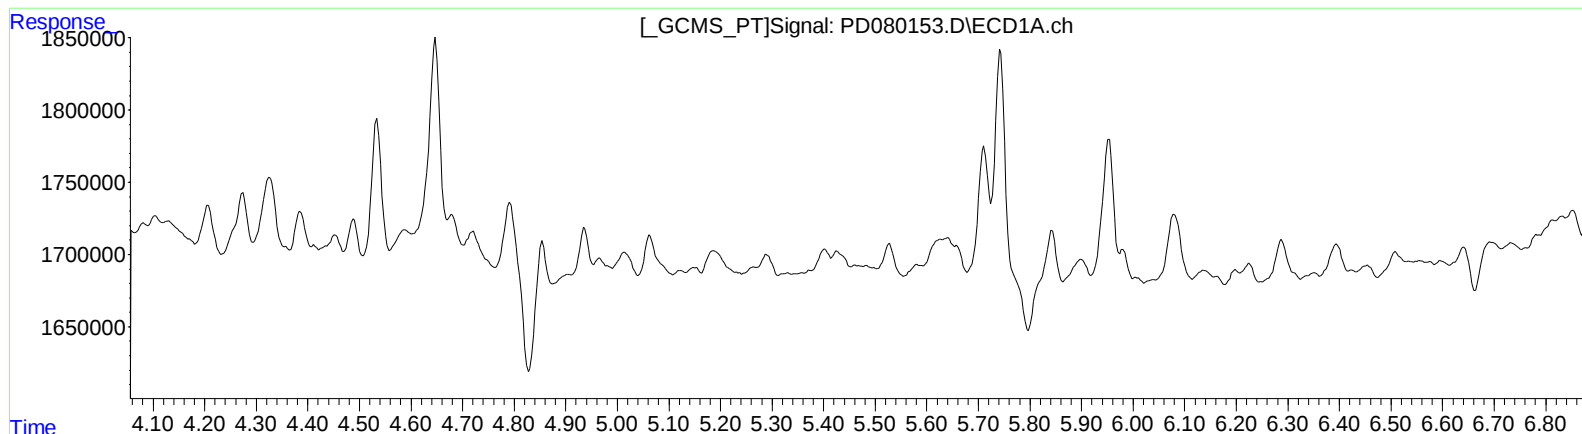

(11) cis-Chlordane (B)

0.000min 0.000 ng/ml

response 0

(11) cis-Chlordane #2 (B)


5.072min 0.637 ng/ml

response 2136772

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD121923\  
Data File : PD080153.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 17 Dec 2023 14:54  
Operator : AR\AJ  
Sample : 05794-04  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 17 20:55:33 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121623CLP.M  
Quant Title : GC Extractables  
QLast Update : Sat Dec 16 03:10:23 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

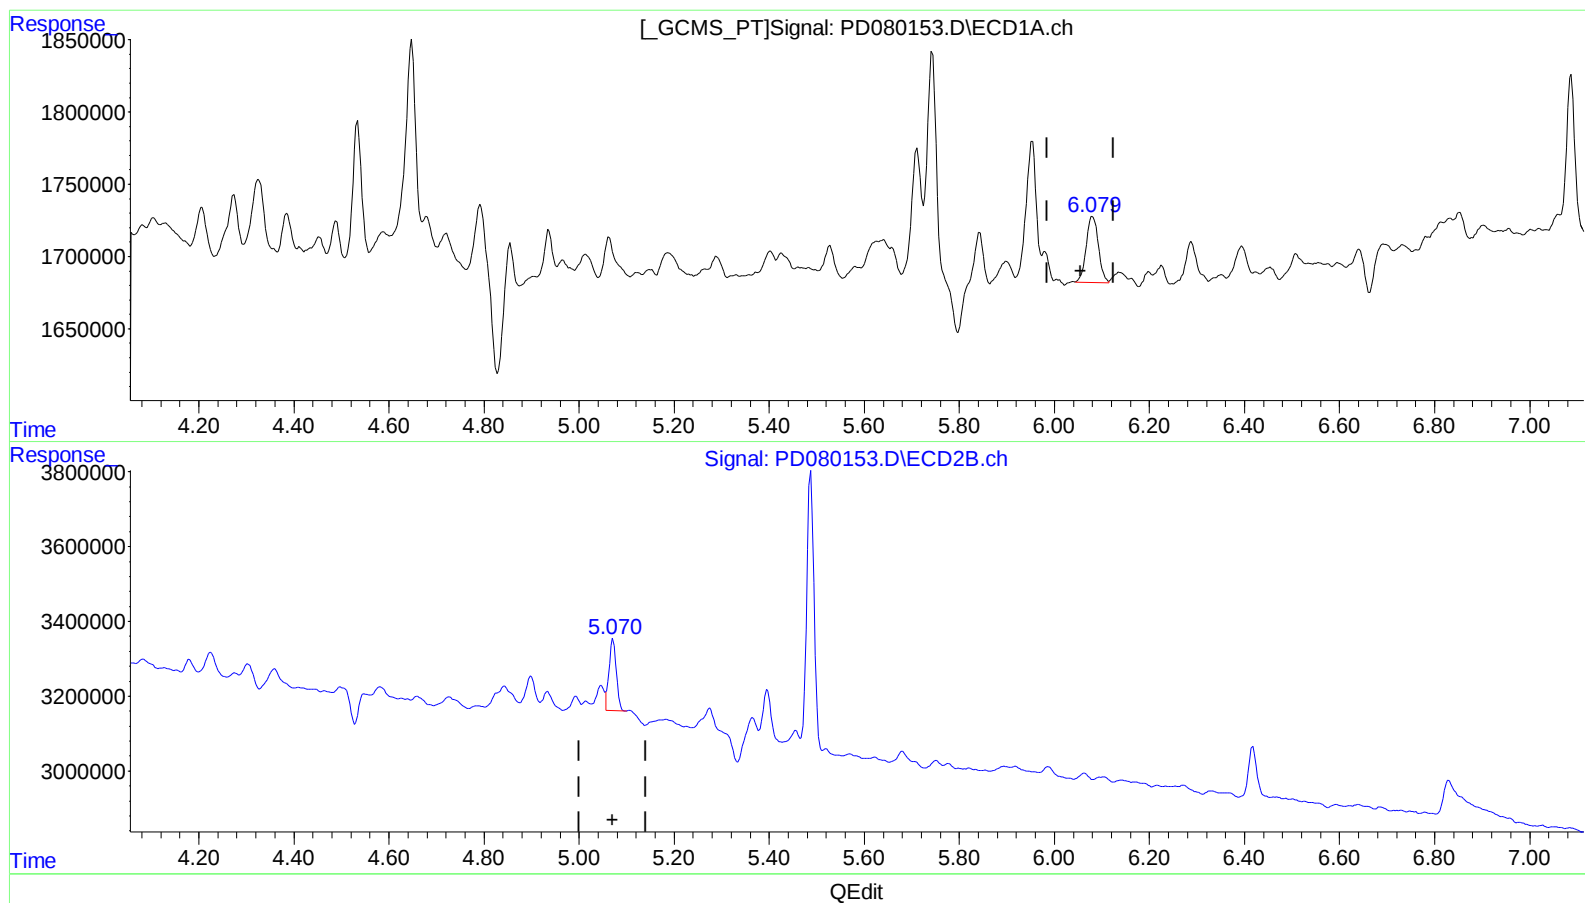

(11) cis-Chlordane (B)

6.079min 0.387 ng/ml m

response 811820

(11) cis-Chlordane #2 (B)

5.072min 0.637 ng/ml

response 2136772

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD121923\  
 Data File : PD080153.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 17 Dec 2023 14:54  
 Operator : AR\AJ  
 Sample : 05794-04  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 17 20:55:33 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121623CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Dec 16 03:10:23 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-------|-------|----------|----------|--------|---------|
| -----                       |       |       |          |          |        |         |
| System Monitoring Compounds |       |       |          |          |        |         |
| 1) SA Tetrachlo...          | 3.567 | 2.801 | 27175959 | 44892196 | 21.285 | 20.189  |
| 2) SA Decachlor...          | 9.113 | 7.942 | 28080728 | 40424660 | 17.466 | 16.842  |
|                             |       |       |          |          |        |         |
| Target Compounds            |       |       |          |          |        |         |
| 11) B cis-Chlor...          | 6.079 | 5.072 | 811820   | 2136772  | 0.387m | 0.637 # |
| -----                       |       |       |          |          |        |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD121923\  
Data File : PD080153.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 17 Dec 2023 14:54  
Operator : AR\AJ  
Sample : 05794-04  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 17 20:55:33 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121623CLP.M  
Quant Title : GC Extractables  
QLast Update : Sat Dec 16 03:10:23 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

