

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121923\
 Data File : PD080164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2023 17:21
 Operator : AR\AJ
 Sample : 05794-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH3Q3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/26/2023
 Supervised By : Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 20:58:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 03:10:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.801	13572635	42562451	10.630	19.142 #
2)	SA Decachlor...	9.097	7.940	44594769	42534336	27.737	17.721 #
Target Compounds							
9)	A Endosulfan I	6.136	5.151	77700213	224.6E6	43.618m	81.926m#
12)	B 4,4'-DDE	6.227	5.259	555.2E6	895.5E6	287.422	285.100
16)	A 4,4'-DDD	6.743	5.812	101.4E6	91147527	73.075	39.642 #
17)	MA 4,4'-DDT	7.060	6.064	3026.3E6	3898.0E6	2047.891	1616.642

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121923\
Data File : PD080164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2023 17:21
Operator : AR\AJ
Sample : 05794-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 20:58:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:10:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

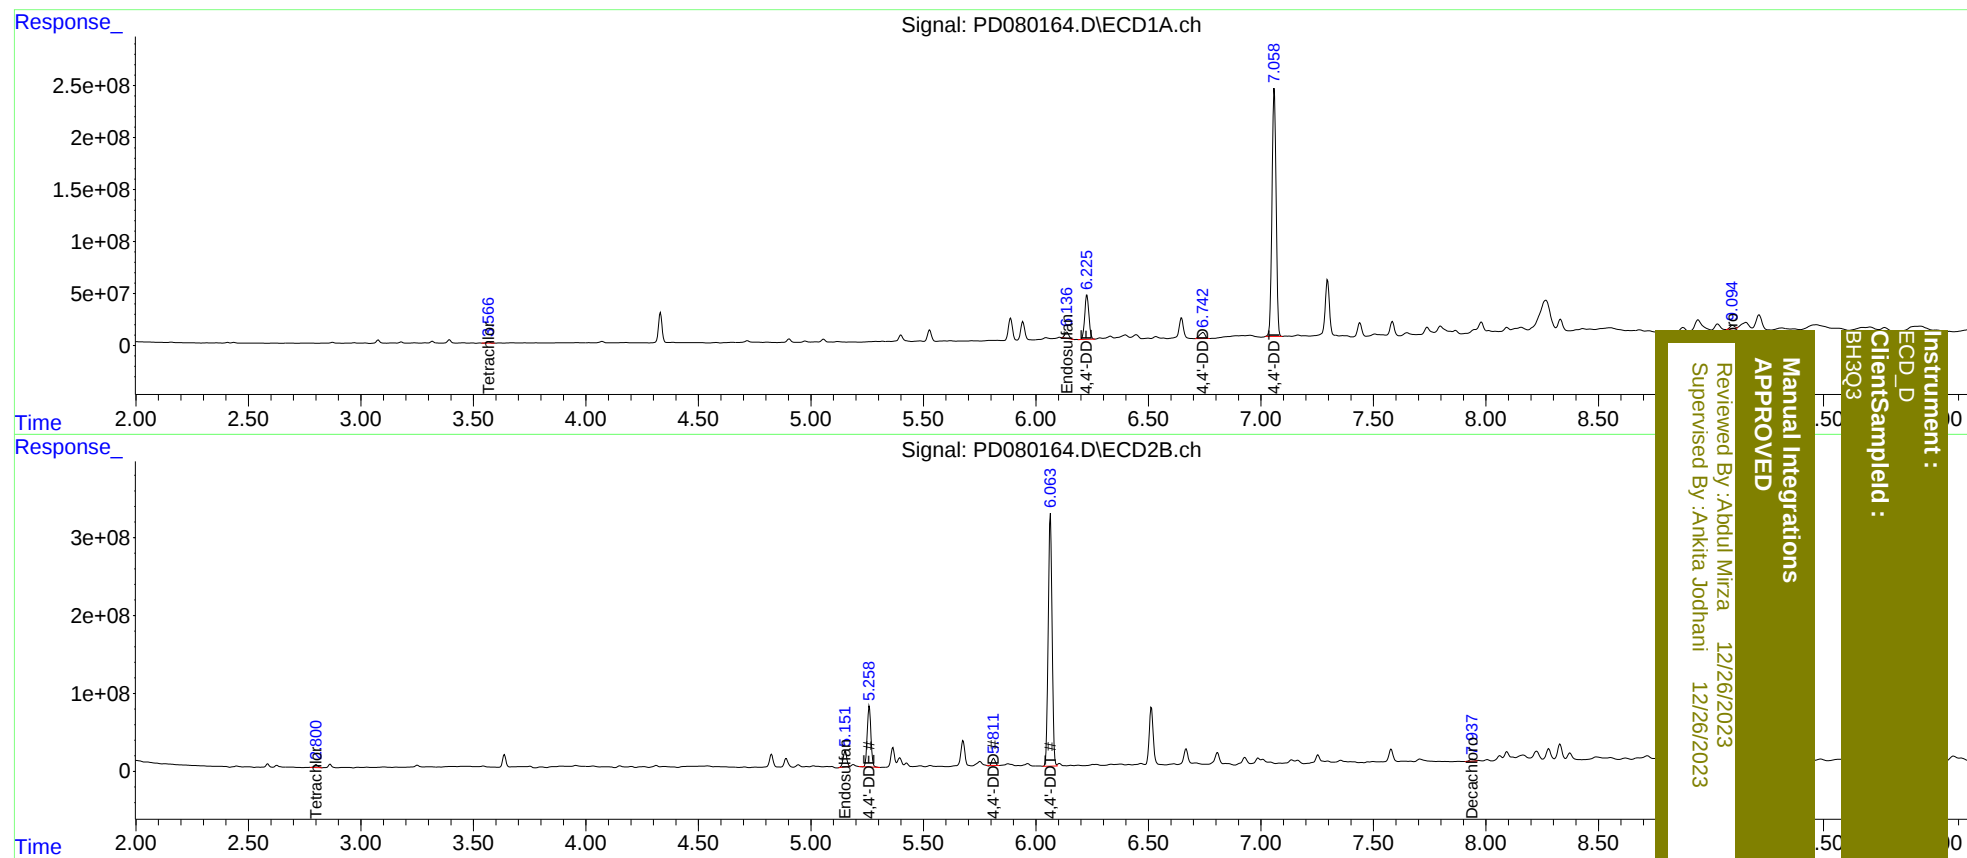

Instrument :
ECD_D
Client Sampled :
BH303
Manual Integrations
APPROVED
Reviewed By : Abdul Mirza 12/26/2023
Supervised By : Ankita Jodhani 12/26/2023