

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121923\
 Data File : PD080166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2023 17:47
 Operator : AR\AJ
 Sample : 05794-11
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH3Q6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/18/2023
 Supervised By : Ankita Jodhani 12/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 20:58:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 03:10:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.568	2.801	11558459	24075210	9.053	10.827
2) SA Decachlor...	9.097	7.941	8219152	34770032	5.112m	14.486 #
Target Compounds						
12) B 4,4'-DDE	6.227	5.259	354.4E6	648.5E6	183.469	206.459m
14) MA Endrin	6.646	5.675	53047870	86156170	33.868m	32.746m
16) A 4,4'-DDD	6.747	5.813	27817609	39582840	20.055	17.216
17) MA 4,4'-DDT	7.059	6.064	259.3E6	397.1E6	175.436	164.679

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121923\
Data File : PD080166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2023 17:47
Operator : AR\AJ
Sample : 05794-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 20:58:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:10:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

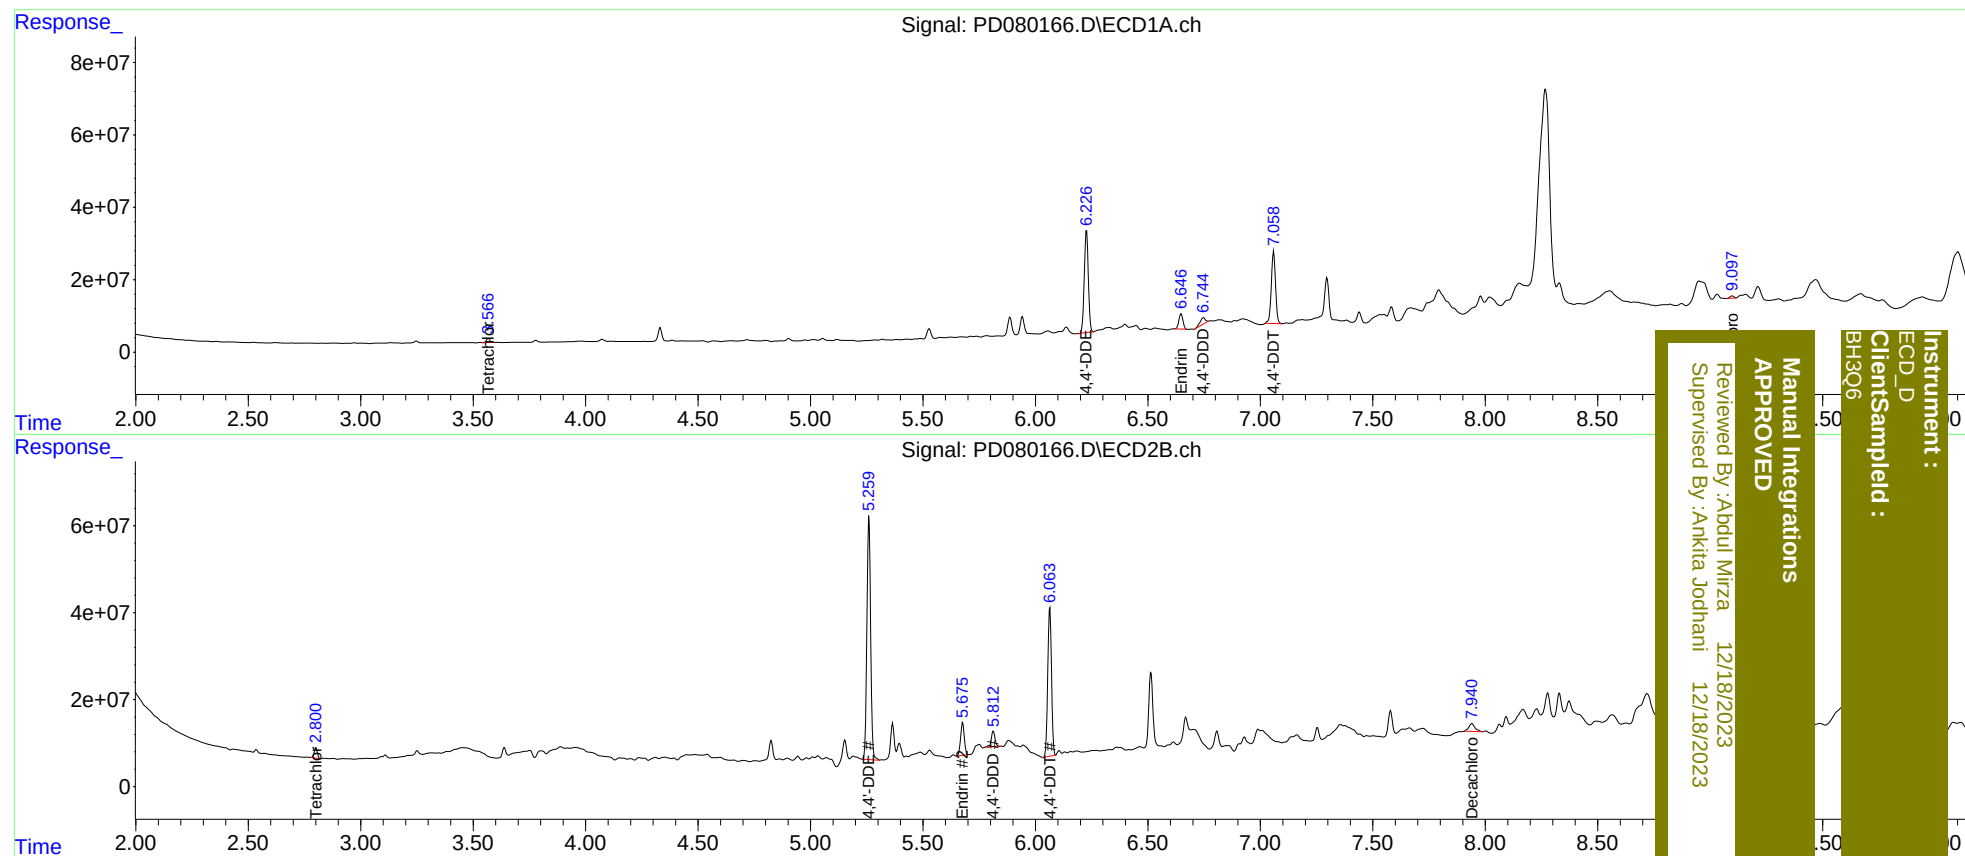

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 12/18/2023
Supervised By: Ankita Jodhani 12/18/2023

Instrument :
ECD_D
Client Sampled :
BH306